

# Structural-Based Uncertainty in Deep Learning Across Anatomical Scales: Analysis in White Matter Lesion Segmentation

Nataliia Molchanova<sup>a,b,c,1</sup>, Vatsal Raina<sup>b,d,2</sup>, Andrey Malinin<sup>e,3</sup>, Francesco La Rosa<sup>a,c,g</sup>, Adrien Depeursinge<sup>a,b</sup>, Mark Gales<sup>d</sup>, Cristina Granziera<sup>h,i,j</sup>, Henning Müller<sup>b,k,l</sup>, Mara Graziani<sup>b</sup>, Meritxell Bach Cuadra<sup>a,c</sup>

<sup>a</sup>*Radiology Department, Lausanne University Hospital (CHUV) and University of Lausanne, Lausanne, Switzerland*

<sup>b</sup>*MedGIFT, Institute of Informatics, School of Management, HES-SO Valais-Wallis University of Applied Sciences and Arts Western Switzerland, Sierre, Switzerland*

<sup>c</sup>*CIBM Center for Biomedical Imaging, Lausanne, Switzerland*

<sup>d</sup>*ALTA Institute, University of Cambridge, United Kingdom*

<sup>e</sup>*Yandex Research, Moscow, Russia*

<sup>f</sup>*Isomorphic Labs, London, United Kingdom*

<sup>g</sup>*Icahn School of Medicine at Mount Sinai, New York, United States of America*

<sup>h</sup>*Translational Imaging in Neurology (ThINK) Basel, Department of Medicine and Biomedical Engineering, University Hospital Basel and University of Basel, Basel, Switzerland*

<sup>i</sup>*Department of Neurology, University Hospital Basel, Basel, Switzerland*

<sup>j</sup>*Research Center for Clinical Neuroimmunology and Neuroscience Basel (RC2NB), University Hospital Basel and University of Basel, Basel, Switzerland*

<sup>k</sup>*Department of Radiology and Medical Informatics, University of Geneva, Geneva, Switzerland*

<sup>l</sup>*TheSense Research and Innovation Center, Lausanne, Sion, Switzerland*

---

<sup>1</sup> Corresponding author.

*Email address: Nataliia (dot) Molchanova (at) unil (dot) ch (Nataliia Molchanova)  
Work phone number and fax do not exist.*

<sup>2</sup> Work was partially during the internship at *b*, the permanent address is *d*.

<sup>3</sup> Work was partially done while working at *e*, new permanent address in *f*.

*April 23, 2024*

---

## Abstract

This paper explores uncertainty quantification (UQ) as an indicator of the trustworthiness of automated deep-learning (DL) tools in the context of white matter lesion (WML) segmentation from magnetic resonance imaging (MRI) scans of multiple sclerosis (MS) patients. Our study focuses on two principal aspects of uncertainty in structured output segmentation tasks. Firstly, we postulate that a good uncertainty measure should indicate predictions likely to be incorrect with high uncertainty values. Second, we investigate the merit of quantifying uncertainty at different anatomical scales (voxel, lesion, or patient). We hypothesize that uncertainty at each scale is related to specific types of errors. Our study aims to confirm this relationship by conducting separate analyses for in-domain and out-of-domain settings. Our primary methodological contributions are (i) the development of novel measures for quantifying uncertainty at lesion and patient scales, derived from structural prediction discrepancies, and (ii) the extension of an error retention curve analysis framework to facilitate the evaluation of UQ performance at both lesion and patient scales. The results from a multi-centric MRI dataset of 334 patients demonstrate that our proposed measures more effectively capture model errors at the lesion and patient scales compared to measures that average voxel-scale uncertainty values. We provide the UQ protocols code at [https://github.com/Medical-Image-Analysis-Laboratory/MS\\_WML\\_uncs](https://github.com/Medical-Image-Analysis-Laboratory/MS_WML_uncs).


*Keywords:* Multiple sclerosis, white matter lesion segmentation, magnetic resonance imaging, deep learning, uncertainty quantification, instance-wise uncertainty, patient-wise uncertainty

---

# Graphical Abstract

## Structural-Based Uncertainty in Deep Learning Across Anatomical Scales: Analysis in White Matter Lesion Segmentation

Nataliia Molchanova, Vatsal Raina, Andrey Malinin, Francesco La Rosa, Adrien Depeursinge, Mark Gales, Cristina Granziera, Henning Müller, Mara Graziani, Meritxell Bach Cuadra

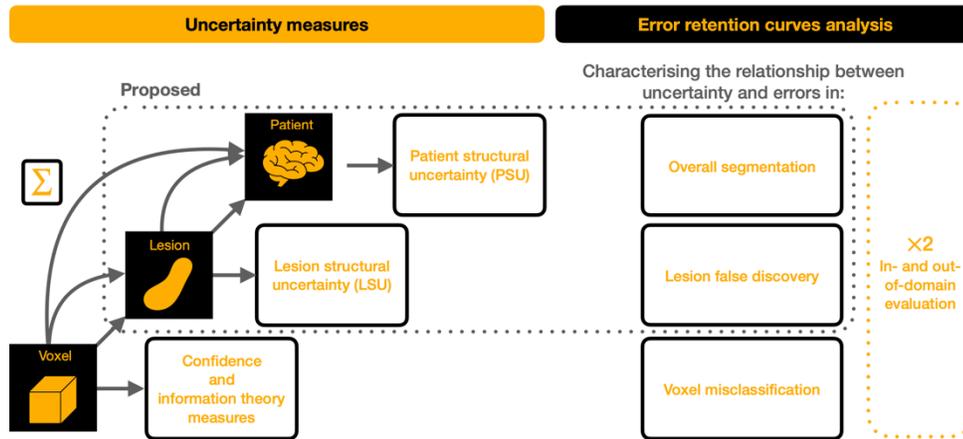

## 1. Introduction

Multiple sclerosis (MS) is a chronic, progressive autoimmune disorder of the central nervous system affecting approximately 2.8 million people worldwide (Walton et al., 2020). The primary characteristics of MS are demyelination, axonal damage, and inflammation due to the breakdown of the blood-brain barrier (Reich et al., 2018; Thompson et al., 2018). The diagnostic criteria for MS include both neurological symptoms observation and magnetic resonance imaging (MRI) examination for the presence of lesions disseminated in time and space (Thompson et al., 2018; Hemond and Bakshi, 2018; Wattjes et al., 2021). White matter lesions (WMLs) are a hallmark of MS, indicating the regions of inflammation in the brain, typically assessed through FLAIR or T1-weighted modalities (Gramsch et al., 2015; Hemond and Bakshi, 2018). On FLAIR scans, WMLs are visible as hyperintense regions with periventricular area, brainstem, and spinal cord being prevalent lesion sites. The size, shape, and count of WMLs vary markedly across patients. While crucial for diagnosis and monitoring, the manual annotation of new and enlarged lesions is a time-consuming and skill-demanding process.

The task of automated WML segmentation has propelled the development of novel image processing techniques for many years (Kaur et al., 2020; Lladó et al., 2012). More recently, algorithms have been boosted by the success of deep learning (DL) in computer vision. DL methods quickly became the state-of-the-art for WML segmentation, providing better performance at faster processing times (Zeng et al., 2020; Spagnolo et al., 2023). Various DL models were explored in application to WML segmentation, with U-Net architecture being the most common model (Spagnolo et al., 2023).

The potential clinical application of DL methods raises safety concerns. These include the black-box nature of such approaches and their susceptibility to variations in test data, known as domain shifts (Reyes et al., 2020). Additionally, such common factors as limited data availability, imperfect annotations, and ground-truth ambiguity due to inter-rater variability further challenge the reliability of DL model predictions, potentially hindering their seamless integration into clinical practice (Begoli et al., 2019). The field of uncertainty quantification (UQ) offers a possibility to tackle this issue by estimating the "degree of untrustworthiness" of model

predictions (Begoli et al., 2019), focusing on two main uncertainty sources (Gawlikowski et al., 2023):

i) data noise, captured by data uncertainty, and ii) training data scarcity or domain shifts, captured by model uncertainty. Talking about high-risk AI applications, the information about the trustworthiness of model predictions is important not only from an engineering perspective, but also for the end-users, e.g. clinicians (Graziani et al., 2022).

Consequently, UQ is gaining popularity within the field of medical image analysis not only as a way to assess prediction trustworthiness. The usage of uncertainty extends beyond quality control to accommodate such applications as improving prediction quality, domain adaptation, active learning, and other applications (Gawlikowski et al., 2023; Faghani et al., 2023; Zou et al., 2023; Lambert et al., 2022c). In medical image segmentation tasks, uncertainty is usually assessed by treating semantic segmentation as pixel/ voxel classification, computing uncertainty for each pixel/voxel prediction. Given the structure of a segmentation model output, it is also possible to explore uncertainty values associated with some region of prediction. Several works explore uncertainty associated with a segmented region of interest, e.g. structure-/ lesion-wise (Roy et al., 2019; Wang et al., 2019; Rottmann et al., 2019; Nair et al., 2020; Lambert et al., 2022b), or for a whole prediction on a patient (Jungo et al., 2020; Whitbread and Jenkinson, 2022).

### *1.1. Related works on uncertainty quantification in multiple sclerosis*

Prior research on UQ for WML segmentation explores different methods, including single-network deterministic methods (McKinley et al., 2020; Lambert et al., 2022a), Monte Carlo Dropout (MCDP) (Gal & Ghahramani, 2015; Nair et al., 2020), batch ensembles (Lambert et al., 2022a). Our previous study investigated the deep ensembles and compared them with the MCDP method, showing the advantage of the first one (Malinin et al., 2022). Utility of a specific UQ method depends on a particular application and available resources (Gawlikowski et al., 2023; Faghani et al., 2023; Zou et al., 2023; Lambert et al., 2022c). Deep ensembles have been subsequently shown to have a higher quality of uncertainty estimates compared to other methods, while being computationally less effective compared to heteroscedastic models or batch ensembles (Gawlikowski et al., 2023; Faghani et al., 2023).

The deep ensemble is a deterministic method as the inference of each member is, thus, the reliability of this UQ method can be studied without a concern about the repeatability of the results.

Using ensemble methods or sampling UQ methods, based on obtaining samples from the posterior distribution, allows for the exploration of various uncertainty measures. Several measures of voxel-scale uncertainty have been explored, including variance, entropy, mutual information (Nair et al., 2020; Lambert et al., 2022b). Our previous study expanded this list by exploring a common negated confidence and more advanced measures of model uncertainty, such as reverse mutual information and expected pairwise Kullback–Leibler divergence (Malinin et al., 2022, Molchanova et al., 2023). Several studies with different UQ methods and measures used, observe that voxel scale uncertainty tends to be the highest at the borders of WMLs, especially big ones (McKinley et al., 2020; Nair et al., 2020; Lambert et al., 2022b; Molchanova et al., 2023; Malinin et al., 2022), resembling partial-volume (Fartaria et al., 2018, 2019) or inter-rater disagreement maps.

In MS, some works have explored uncertainty associated with a segmented region of interest, i.e. at the lesion scale (Nair et al., 2020; Lambert et al., 2022b; Molchanova et al., 2023). The pioneering study (Nair et al., 2020) suggested computing a *log-sum* of voxel-scale uncertainties across a predicted lesion region, using different voxel-scale uncertainty maps. Analogously, mean average voxel uncertainty values across the lesion region were explored (Lambert et al., 2022a). Lambert et al., 2022a has shown the advantages of structural UQ based on graph neural networks over voxel aggregation methods. Our prior research (Molchanova et al., 2023) demonstrated that lesion-scale uncertainty, computed through disagreement in structural predictions, is more effective at identifying false-positive lesions than aggregating voxel-scale uncertainties. In the context of MS lesion segmentation the patient-scale uncertainty is less explored.

Besides these various proposed measures, prior works proposed different ways to compare uncertainty measures. Ideally, a high uncertainty score should highlight the predictions that are the most likely to be wrong. Hence, we expect a good quality uncertainty measure to reflect the increased likelihood of an erroneous prediction and thus correlate with model mistakes. For classification tasks, a calibration of uncertainty is measured to

assess its quality, similarly the uncertainty quality can be compared at the voxel scale. At the lesion-/ patient- scales the calibration metrics are not explicitly defined. When investigating lesion-scale measures, Nair et al., 2020 looked into uncertainty-based prediction filtering as a means to correlate uncertainty and false positive errors, and Lambert et al., 2022a used accuracy-confidence curves. Our previous work redefines an error retention curve analysis to quantify the relationship between uncertainty and lesion detection errors (Molchanova et al., 2023). Prior to that the error retention curve analysis has been explored to compare classification or segmentation pixel-/ voxel-scale uncertainty measures for various tasks as a way to quantify its relationship with an error / quality metric of a choice (Malinin, 2019; Malinin et al., 2022; Mehta et al., 2022). This is a necessary analysis for various practical clinical implementations, including a signaling uncertainty-based system to warn medical specialists about the potential errors in automatic predictions, automatic uncertainty-based filtering of errors, or active learning where the hardest, i.e. most likely erroneous examples need to be selected.

Various studies on UQ for WML segmentation use similar U-net-like deep learning models (Ronneberger et al., 2015; Çiçek et al., 2016; Nair et al., 2020; Malinin et al., 2022; Lambert et al., 2022a), which have been widely explored in application to the MS lesion segmentation task (Kaur et al., 2020; Zeng et al., 2020; La Rosa et al., 2020; Spagnolo et al., 2023). While there is an agreement about the DL model, studies were conducted on various datasets, predominantly private ones. There has not been a public benchmark dataset for the UQ methods evaluation within the context of WML segmentation before the Shifts 2.0 Challenge (Malinin et al., 2022).

## 1.2. *Our contributions*

This study extends our previous work (Molchanova et al., 2023) and introduces advancements in uncertainty quantification (UQ) methods, focusing on MRI segmentation across voxel, lesion, and patient scales. We introduce a novel patient-scale uncertainty measure that leverages ensemble member disagreement to more accurately identify segmentation errors. To compare patient-scale measures, we redefine the error retention curves analysis, enabling a better understanding of their performance in detecting poor segmentation quality. Our quantitative evaluation is conducted in both

in-domain and out-of-domain settings to mirror the diversity of MRI data coming from different studies, medical centers, and scanners. Additionally, this research provides a comparison of uncertainty measures across different anatomical scales, highlighting their capacity to detect voxel misclassification, lesion false discovery, and general segmentation inaccuracies, considering clinically-relevant applications. The proposed UQ framework is specifically tailored for white matter lesion (WML) segmentation on FLAIR MRI scans.

Our contributions include:

- Proposing the error retention curves analysis for instance-detection tasks, enabling an evaluation of lesion-scale UQ methods in their ability to capture lesion false detection errors.
- Proposing a patient-scale uncertainty measure, a novel approach for WML segmentation, enhancing the understanding of overall segmentation failure.
- Proposing the extension of the error retention curves analysis for patient-scale to compare the ability of different uncertainty measures to capture overall segmentation quality.

## **2. Materials and methods**

### *2.1. Data*

The study setup was designed as a part of the Shifts Challenge (Malinin et al., 2022) specifically for the exploration of uncertainty quantification across shifted domains. For the setup creation, we used three publicly available datasets and a single private one. Despite the availability of various modalities in the Shifts data, this study uses only FLAIR (Gramsch et al., 2015) scans and their manual WML annotations. Regardless of the medical center, each FLAIR scan underwent a common pre-processing pipeline comprising denoising (Coupé et al., 2008), skull stripping (Isensee et al., 2019), bias field correction (Tustison et al., 2010), and interpolation to  $1mm$  iso-voxel space. Manual WML annotations formed by max-voting or by consensus between several experts depending on the study were used as ground truth.

Data is separated into in- and out-of-domain subsets where the domain shift is provided by the difference in study, medical center, scanner model, annotators, and MS stages. In-domain data comprises the training (Train, 33 scans), validation (Val, 7 scans), and in-testing dataset ( $Test_{in}$ , 33 scans) sets. Out-of-domain data includes the 99 pure testing scans ( $Test_{out}$ , 99 scans). Particular data split into in- and out-of-domain sets was designed to maximize the drop of model performance in lesion segmentation in the out-of-domain setting (Malinin et al., 2022). To prove the replicability of our work, we extend this existing public benchmark by including a large in-house dataset ( $Test_{private}$ , 162 scans) collected in the Basel University Hospital, Switzerland (Granziera, C., 2018). The dataset was processed similarly to the Shifts data. While  $Test_{private}$  should be treated as an out-of-domain, the lesion profiles overlap with both  $Test_{in}$  and  $Test_{out}$  (see Figure 1).

Information about data sources, metadata, and data splits is provided in Table 1. Figure 1 illustrates some differences between domains brought by variations in MS stage distributions and scanner changes, affecting the lesion characterization and intensity features, respectively. Other factors, such as changes in study design, lesion annotators, scanner operators, may also contribute to the domain shift.

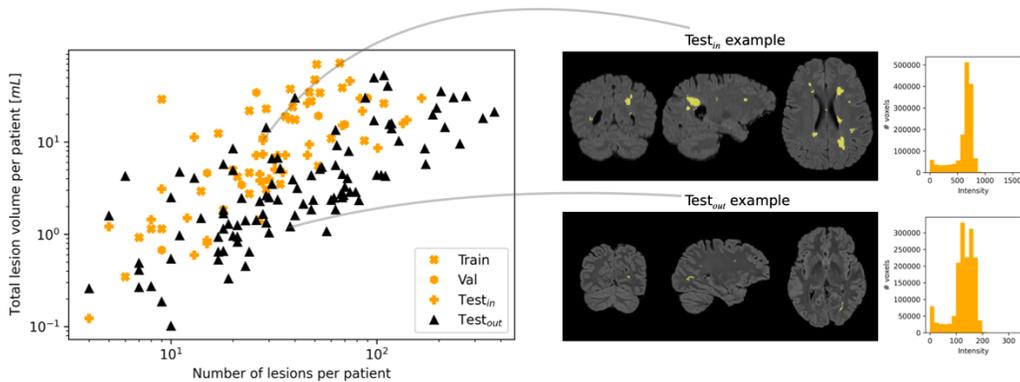


Figure 1: Illustration of the domain shift between the in-domain datasets (Train, Val,  $Test_{in}$ ) and the out-of-domain dataset ( $Test_{out}$  and  $Test_{private}$ ) brought by the differences in the MS stages and medical centers. On the left, the plot of the total lesion volume in milliliters versus the number of lesions per scan for in-domain (orange) and out-of-domain (black and gray) sets reveals the difference in the lesion load (as a proxy to an MS stage) between different domains. On the right, typical examples from the  $Test_{in}$  and  $Test_{out}$  sets to illustrate the difference in the lesion load, as well as the intensity differences brought by the change of the medical center (i.e. scanner, technicians, annotators, and other parameters contributing to the domain shift).

Domain	In-domain			Out-of-domain	
	Train	Val	Test <sub>in</sub>	Test <sub>out</sub>	Test <sub>private</sub>
Source	Carass et al. (2017), Commowick et al. (2018)			Lesjak et al. (2017), Bonnier et al. (2014)	Basel University Hospital (Granziera, C., 2018)
Scanners	Siemens (Aera 1.5T, Verio 3.0T), GE Disc 3.0T, Philips (Ingenia 3.0T, Medical 3.0T)			Siemens Magnetom Trio 3.0T	Siemens Magnetom Prisma 3.0T
M:F ratio range	0.21-0.4			0.23-0.70	0.68
MS stages	RR, PP, SP			CIS, RR, SP, PP	RR, PP, SP
# raters	2 or 7			consensus or 3	consensus
Inter-rater agreement (Dice score)	0.63 and 0.71			0.78	-
Set name	Train	Val	Test <sub>in</sub>	Test <sub>out</sub>	Test <sub>private</sub>
# scans	33	7	33	99	162
# lesions per scan, Q2 (IQR)	34 <sub>(20-50)</sub>	26 <sub>(19-61)</sub>	30 <sub>(15-47)</sub>	39 <sub>(20-77)</sub>	63 <sub>(25-88)</sub>
Total lesion volume per scan, Q2 (IQR) [mL]	12.5 <sub>(3.1-27.8)</sub>	15.5 <sub>(4.0-24.7)</sub>	7.2 <sub>(3.7-11.3)</sub>	2.7 <sub>(1.3-7.3)</sub>	7.4 <sub>(2.4-14.3)</sub>

Table 1: Data splits and meta information. MS stages are clinically isolated syndrome (CIS), relapsing remitting (RR), primary progressive (PP), and secondary progressive (SP).

## 2.2. Uncertainty quantification

This work implements deep ensembles (Lakshminarayanan et al., 2017) for UQ by training multiple networks with identical architecture but different random seed initializations. The random seed controls several factors, for

instance, weights initialization, training sample selection, random augmentations, and stochastic optimization algorithms. Although each ensemble member has distinct model weights, they all stem from the same posterior distribution. This causes varied predictions among ensemble members for the same input example. The spread or variation in these predictions serves as an uncertainty estimate.

### 2.2.1. *Uncertainty quantification at different anatomical scales*

In an image segmentation task, a class prediction is not a single value but an image-size map. Thus, the disagreement between the ensemble members can be quantified not only for each voxel of the prediction but also for a subset of its elements. For WML segmentation, the model prediction is a 3D probability map. We can quantify the uncertainty associated with the decision taken in each voxel, thus obtaining another 3D map with voxel-scale uncertainty values. We can also quantify uncertainty associated with a set of predictions within a region of a particular lesion, thus obtaining an uncertainty score for each predicted lesion. Similarly, we can quantify uncertainty for the whole patient. We implement several uncertainty measures at each anatomical scale (voxel, lesion, or patient). The exact mathematical formulation for the previous existing and proposed UQ measures are summarized in Table 2 and described hereafter.

**Voxel-scale uncertainty measures.** Perceiving segmentation as a classification of each voxel of an image, one could use uncertainty measures available for classification tasks to quantify uncertainty for per-voxel predictions. The common uncertainty measures in this case will be negated confidence and information theory measures such as entropy of expected, expected entropy, or mutual information which respectively depict different *total*, *data*, and *knowledge* uncertainty.

**Lesion-scale uncertainty measures.** Given a WML segmentation task, we can compute a single uncertainty score for each predicted connected component, *i.e.* lesion. Differently from previous measures that aggregate voxel-scale uncertainties (Nair et al., 2020; Lambert et al., 2022a), our previous work (Molchanova et al., 2023) proposes a novel lesion-scale uncertainty defined directly through the disagreement between the lesion structural predictions of ensemble members. We hypothesize that looking at

the disagreement in structural predictions, i.e. predicted lesion regions, might be more beneficial for the discovery of false positive lesions.

To define our proposed measure we should consider the ensemble of  $M$  models, where each member model is parametrized by weights  $\theta^m, m = 0, 1, \dots, M-1$ . The ensemble probability prediction is obtained by computing a mean average across members. Then, the binary lesion segmentation mask is obtained by applying a threshold  $\alpha$  to the softmax ensemble prediction, where  $\alpha$  is chosen based on the Dice similarity coefficient maximized on the validation dataset. Analogously, by applying the threshold  $\alpha$  to the softmax predictions of each of the ensemble models, we can obtain the binary lesion segmentation masks predicted by each model  $m$  in the ensemble. Let  $L$  be a *predicted lesion* that is a connected component from the binary segmentation map obtained from the ensemble model; and  $L^m$  is the *corresponding lesion* predicted by the model  $m$ , determined as the connected component on the binary segmentation map predicted by the  $m^{th}$  member with maximum intersection over union (IoU) with  $L$ . If the softmax probability threshold is optimized for each member model separately based on the highest Dice score, the resulting thresholds will be different from  $\alpha$  and will be member-specific:  $\alpha^m, m = 0, 1, \dots, M-1$  instead of  $\alpha$ . Then, the binary segmentation maps obtained with  $\alpha^m$  will lead to different *corresponding lesion* regions, called  $L^{m,+}$ . Then, the proposed measures lesion structural uncertainty (LSU) measures are defined as follows:

$$LSU = 1 - \frac{1}{M} \sum_{m=0}^{M-1} IoU(L, L^m), \quad (1)$$

and

$$LSU^+ = 1 - \frac{1}{M} \sum_{m=0}^{M-1} IoU(L, L^{m,+}). \quad (2)$$

**Patient-scale uncertainty measures.** Patient-scale uncertainty offers the most compact way of uncertainty representation considering the clinical practice, that is presenting a single uncertainty score per patient. Analogously to the lesion scale, the patient-scale uncertainty can be computed by averaging voxel or lesion uncertainties.

Using similar reasoning as for the lesion scale, we propose a patient-scale measure analogous to LSU (Equation (1)), where instead of the lesion region  $L$  the total segmented lesion region is used.

To define these measures, let  $S$  be a set of voxels predicted as lesion class by the ensemble model,  $S^m$  - set of voxels predicted as lesion class by the  $m^{th}$  member model in the ensemble, and  $S^{m,+}$  is the same, but obtained with the member-specific threshold  $\alpha^m$ . Then, the proposed patient structural uncertainty measures are defined as:

$$PSU = 1 - \frac{1}{M} \sum_{m=0}^{M-1} IoU(S, S^m), \quad (3)$$

and

$$PSU^+ = 1 - \frac{1}{M} \sum_{m=0}^{M-1} IoU(S, S^{m,+}). \quad (4)$$

- a) **Voxel-scale uncertainty measures** computed for each pixel  $i \in B$  of an input scan  $\mathbf{x}$  ( $B$  is a set of voxels defining the brain region),  $\mathbf{y}$  - targets,  $c = 0, 1, \dots, C-1$  is the class ( $C = 2$  for binary segmentation),  $P(y_i = c | \mathbf{x}, \theta^m)$  is a predictive posterior of model  $m$  parametrized by weights  $\theta^m$  in the ensemble of  $M$  models, and  $P(x) = \frac{1}{M} \sum_{m=0}^{M-1} P(x, \theta^m)$  is for the whole ensemble model.

<p>Negated confidence</p> $NC_i = -\operatorname{argmax}_{c=0, \dots, C-1} \frac{1}{M} \sum_{m=0}^{M-1} P(x, \theta^m)$
<p>Entropy of expected</p> $EoE_i = - \sum_{c=0}^{C-1} P(x) \log P(x)$
<p>Expected entropy</p> $ExE_i = - \frac{1}{M} \sum_{m=0}^{M-1} \sum_{c=0}^{C-1} P(x, \theta^m) \log P(x, \theta^m)$
<p>Mutual information</p> $MI_i = EoE_i - ExE_i$

- b) **Lesion-scale uncertainty measures** computed for each *predicted lesion*  $L$ , that is a connected component on the ensemble-predicted binary segmentation map. The last is obtained by applying a threshold  $\alpha$  to the softmax ensemble prediction  $P(\mathbf{y} = \mathbf{1} | \mathbf{x}) = \{P(y_i = 1 | \mathbf{x}), i \in B\}$ , where  $\alpha$  is chosen based on the Dice similarity coefficient maximized on the validation dataset.  $L^m$  is the *corresponding lesion* predicted by the  $m^{\text{th}}$  member model, determined as the connected component on the binary segmentation map predicted by the  $m^{\text{th}}$  member (threshold  $\alpha$  applied to  $P(\mathbf{y} = \mathbf{1} | \mathbf{x}, \theta^m), m = 0, 1, \dots, M-1$ ) with maximum intersection over union (IoU) with  $L$ . If the softmax probability threshold is optimized based on the highest Dice score for each member model separately, the resulting thresholds will be different from  $\alpha$  and will be member-specific:  $\alpha^m, m = 0, 1, \dots, M-1$  instead of  $\alpha$ . Then, the binary segmentation maps obtained by applying  $\alpha^m$  to  $P(\mathbf{y} = \mathbf{1} | \mathbf{x}, \theta^m), m = 0, 1, \dots, M-1$  will lead to different corresponding lesion regions, called  $L^{m,+}$ .

<p>Voxel uncertainties aggregation via mean average <math>\overline{EoE}_L = \frac{1}{ L } \sum_{i \in L} EoE_i</math>.</p> <p>Analogously, <math>\overline{ExE}_L, \overline{NC}_L, \overline{MI}_L</math> are defined.</p>
<p><b>Proposed</b> lesion structural uncertainty (LSU)</p> $LSU = 1 - \frac{1}{M} \sum_{m=0}^{M-1} IoU(L, L^m) \text{ and } LSU^+ = 1 - \frac{1}{M} \sum_{m=0}^{M-1} IoU(L, L^{m,+})$

- c) **Patient-scale uncertainty measures** computed for patient.  $S$  is a set of voxels predicted as lesions by the ensemble model,  $S^m$  is a set of voxels predicted as lesions by the model  $m$ , and  $S^{m,+}$  is the same, but obtained with the member-specific threshold  $\alpha^m, m = 0, 1, \dots, M-1$ .  $W$  - set of lesions predicted by the ensemble model.

<p>Voxel uncertainties aggregation via mean average <math>\overline{EoE}_B = \frac{1}{ B } \sum_{i \in B} EoE_i</math>.</p> <p>Analogously, <math>\overline{ExE}_B, \overline{NC}_B, \overline{MI}_B</math> are defined.</p>
<p>Proposed lesion uncertainties aggregation via mean average <math>\overline{LSU} = \frac{1}{ W } \sum_{i \in W} LSU_i</math>. Analogously, <math>LSU^+</math> is defined.</p>
<p><b>Proposed</b> patient structural uncertainty (PSU)</p> $PSU = 1 - \frac{1}{M} \sum_{m=0}^{M-1} IoU(S, S^m) \text{ and } PSU^+ = 1 - \frac{1}{M} \sum_{m=0}^{M-1} IoU(S, S^{m,+})$

Table 2: Definitions of uncertainty measures at three anatomical scales: voxel, lesion, and patient.

### 2.3. Quantitative evaluation of uncertainty measures

Uncertainty has a relation to errors made by a model: ideally, a higher uncertainty expresses an increased likelihood of erroneous prediction. For each of the anatomical scales: voxel, lesion, and patient, the “error” definition can vary. For example, a voxel-scale error can be simply defined as a voxel misclassification, a lesion-scale error can be defined as a lesion misdetection, and a patient-scale error can be a summary of voxel errors. In this work, we want to compare voxel-, lesion-, and patient-scale uncertainty measures in terms of their ability to capture errors of different kinds. For this, we use an error retention curves analysis (Malinin, 2019; Malinin et al., 2022; Mehta et al., 2022), previously introduced only for voxel-scale uncertainty, and extended for lesion and patient scales in this work.

#### 2.3.1. Error and quality metrics

We start by defining errors on the voxel and lesion scale as well as quality metrics used in this work for model performance characterization and error retention curves analysis.

**Voxel-scale errors.** Similarly to a classification task, the errors at the voxel scale will include false positives and negatives (FP and FN, respectively). Based on FP, FN, true positives (TP), and true negatives (TN), one derives metrics like true positive rate (TPR) and positive predictive value (PPV), which measure correctly classified voxels against ground truth or predicted lesions, respectively. To evaluate both error types, we use the  $F_1$  score, also known as the Dice similarity score (DSC) in image processing. However, it is well known that the DSC metric suffers from a bias to the occurrence rate of the positive class, i.e. lesion load, jeopardizing the comparison of results. We thus additionally utilize the normalized DSC (nDSC) (Raina et al., 2023) for the model evaluation. In a nutshell, nDSC scales the precision at a fixed recall rate to tackle the lesion load bias.

**Lesion-scale errors.** Analogously, true positive, false positive, and false negative lesions (TPL, FPL, FNL) can be defined if the criteria for lesion (mis)detection are given. While some studies accept minimal overlap for detection (Nair et al., 2020; Carass et al., 2017; La Rosa et al., 2020), we apply a 25% intersection over the union threshold for a predicted lesion to be considered a TPL. For the FNL definition, we consider a zero overlap with the

prediction. A FNL is a ground truth lesion that has no overlap with predictions. Metrics derived from TPL, FPL, and FNL include Lesion TPR, PPV, and  $F_1$ , further referred to as LTPR, LPPV,  $LF_1$ . The differences at the voxel scale include: i) uncertainty cannot be quantified for FNLs, as they are not predicted lesions; ii) it is not possible to define a true negative lesion. The metrics definitions can be found in Appendix A.

### 2.3.2. Error retention curve analysis

The error retention curves (RCs) (Malinin, 2019; Malinin et al., 2022; Mehta et al., 2022) assess the correspondence between a chosen uncertainty measure and an error or a quality metric. By quantifying this correspondence for various uncertainty measures we can choose a measure that is better at pointing out errors in model predictions. This is relevant for the clinical applications, where uncertainty constitutes a signaling system requiring human verification.

Compared to the uncertainty calibration analysis (Gawlikowski et al., 2023), error RCs only take into account the ranking of uncertainty values within a particular scan, thus, avoiding uncertainty values scaling present in the calibration metrics. Additionally, they allow for the choice of a quality metric w.r.t. to which the uncertainty measure is compared. Thus, allowing for extending their definition to different scales, e.g. lesion or patient. Moreover, compared to calibration metrics, the RC analysis allows us to estimate the upper and lower bounds of the uncertainty-robustness performance.

**Voxel-scale DSC-RC.** Analogously to our previous investigation (Molchanova et al., 2023), we use voxel-scale retention curves to quantify the average across patients correspondence between per-voxel uncertainty and DSC, *i.e.* per-voxel misclassification errors of different kinds: either FP or FN. The voxel-scale RC for a single patient is built by sequentially replacing a fraction  $\tau$  of the most uncertain voxel predictions within the brain mask with the ground truth and re-computing the DSC. If one measure has a better ability to capture model errors than another measure, then the most uncertain voxels will be faster replaced with the ground truth and the DSC-RC will grow faster. Thus, the area under the DSC retention curve (DSC-RC), further referred to as DSC-AUC can be used to compare different uncertainty measures in their ability to capture model segmentation errors. Additionally,

it is possible to estimate lower and upper bounds of performance by building *random* and *ideal* RCs. For a random RC, we assign random uncertainty values to each voxel of predictions. For the ideal one, a zero uncertainty is assigned to true positive and negative (TP and TN) voxels while false positive and negative (FP and FN) voxels have an uncertainty of 1. To build the RCs, we use  $\tau = 2.5 \cdot 10^{-3}$ . An illustrative explanation of a voxel-scale RC can be found in Figure 2.

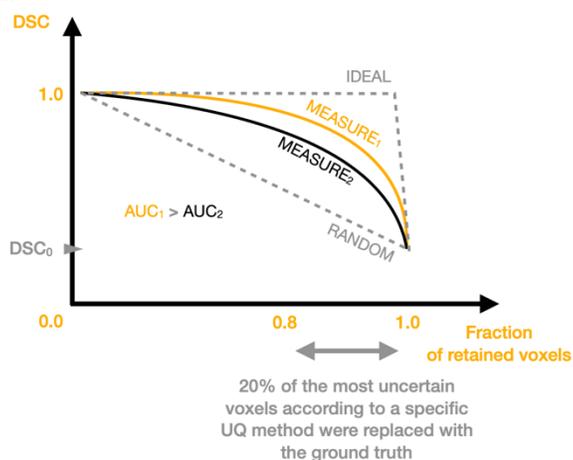


Figure 2: An illustration of a retention curve (RC) on the voxel scale for assessing the correspondence between an uncertainty (MEASURE<sub>1</sub> and MEASURE<sub>2</sub>) and model performance measured by DSC in a patient. When all the voxels are retained the  $y$ -value is equal to the original DSC of the model on the subject ( $DSC_0$ ). IDEAL and RANDOM lines built using ideal and random uncertainty measures constitute the upper and lower bounds of the uncertainty-robustness performance.

**Lesion-scale LPPV-RC (proposed).** In our previous investigation (Molchanova et al., 2023) we proposed an extension of the error RC analysis to the lesion scale through LF1-RC. LF1-RC assesses the correspondence between lesion-scale uncertainty and errors in lesion detection within a patient. As defined in Section 2.3.1, the LF1 is reflective of both FNL and FPL. However, uncertainty cannot be defined for FNLs as they are not predicted, but ground-truth lesions. Thus, LF1-RCs are more suitable for the comparison of different models or uncertainty quantification methods, for which the number of FNL can vary. However, for the comparison of lesion-

scale uncertainty measures, where the number of FNL does not change, the LPPV-RC analysis is sufficient. Thus, we propose the LPPV-RC assesses the correspondence between lesion-scale uncertainty and lesion false positive errors within a patient. Intuitively, this analysis helps to understand which uncertainty measure is the best at pointing to false positive lesions.

Building a LPPV-RC for a patient starts with computing the number of TPL and FPL, *i.e.*  $\#_{TPL}$  and  $\#_{FPL}$ , and uncertainty values for each of these lesions. Further, the most uncertain lesions are sequentially replaced with TPL, and LPPV is recomputed. Analogously to the voxel scale, if a lesion-scale uncertainty measure has a better ability to capture FPL than another measure, then FPL will be replaced faster and the curve will grow faster. Thus, the area under the LPPV-RC, that is LPPV-AUC, can be used to compare different measures in their ability to capture FPL detection errors. As each patient has a different number of predicted lesions, to obtain an average across the dataset LPPV-AUC, we first need to interpolate all LPPV-RCs to a similar set of retention fractions. For this, we use a piecewise linear interpolation and a set of retention fractions similar to the voxel scale. Additionally, similarly to the voxel scale, the ideal and random RCs are built. The ideal curve is built by considering all TPLs having an uncertainty of 0 and all FPLs having an uncertainty of 1. The random curve is built by using random uncertainties for each of the lesions.

**Patient-scale DSC-RC (proposed).** In this work, we propose a way to extend an error RCs analysis to the patient scale to assess the correspondence between patient-scale uncertainty measures and overall prediction quality in a patient. We use DSC as a measure of overall segmentation quality. Then, a patient-scale DSC-RC is built by sequentially excluding the most uncertain patients, that is replacing their DSC with 1.0, and recomputing the average across the dataset DSC. Similarly to the voxel and lesion scales, the area under the patient-scale DSC-RC is used to compare the ability of different patient-scale uncertainty measures to capture patients with a greater amount of erroneous predictions. In analogy to the voxel and lesion scales, we want to assess the upper and lower bounds of the performance with ideal and random patient-scale DSC-RCs. To build a random curve we assign random uncertainties to each of the patients. To build the ideal curve, we use a negated DSC score as an uncertainty measure,

as we want ideal uncertainty to point to the most erroneous examples in terms of DSC.

**Statistical testing.** For the voxel and lesion scales, the error retention curves analysis, namely DSC-RC and LPPV-RC, are computed per patient. Therefore, when comparing different uncertainty measures across each other, one can assess the differences in AUC distributions across measures, *e.g. statistics*. For the patient scale, DSC-RC is computed per dataset (by iterative replacement of the most uncertain patients). Nevertheless, it is possible to estimate the bootstrap confidence intervals by treating the patient-scale DSC-RC as a statistic itself. Thus, to conduct the measures ranking for the patient-scale uncertainty measures, we compare the mean patient-scale DSC-AUC, paying attention to the corresponding confidence intervals.

### 2.3.3. *Patient-scale uncertainty as a proxy for segmentation quality*

In addition to the information brought by the error RC, we would like to study if a patient-scale uncertainty can serve as a proxy to the model segmentation quality, measured by DSC. For this, we compute Spearman's correlation coefficient  $\rho$  between the DSC and uncertainty values. The Spearman's correlation is computed for different test sets separately, and then jointly. The joint correlation coefficient should show if the uncertainty measure can be used as a proxy for the segmentation quality regardless of the domain shift. This might be particularly useful for the scenario where the domain shift is unknown.

## 2.4. *WML segmentation models*

For this study, we consider two models based on a 3D U-Net architecture. Similar 3D-U-net-based models have been previously used for WML segmentation and compared to other approaches (Kaur et al., 2020; Zeng et al., 2020; La Rosa et al., 2020; Spagnolo et al., 2). Furthermore, our choice is supported by the fact that the same model has been extensively used previously for UQ exploration within the same WML segmentation task in MS (McKinley et al., 2020; Nair et al., 2020; Malinin et al., 2022; Lambert et al., 2022a; Lambert et al., 2022b). The first model is the baseline model from the Shifts 2.0 Challenge (Malinin et al., 2022) dedicated to UQ for WML segmentation. The second model is a self-configuring nnU-Net architecture

(Isensee et al., 2020). Both models are ensembles with 5 members, where each member is a 3D U-Net model (Ronneberger et al., 2015; Çiçek et al., 2016). There are several crucial differences between the Shifts Baseline (SB) U-Net and the nnU-Net models: i) architecture, i.e SB has the depth reduced by one and, thus, less trainable parameters; ii) loss function, i.e. Focal-Dice loss for SB and cross-entropy and Dice loss for nnU-Net; iii) deep supervision is utilized by nnU-Net, compared to SB; iv) input, SB's input are patches of the size  $96 \times 96 \times 96$  cropped from the brain using a sequence of transforms, while nnU-Net uses patches  $112 \times 160 \times 128$  cropped around the whole brain. Both models represent public benchmarks and their training and inference code is available online <sup>4</sup>. For the SB model, the only difference, compared to the original model, is an addition of 2 more ensemble members, obtained using the original training code. For the nnU-Net model, we used a "3d\_fullres" configuration, we ensured the consistency of training and validation examples across folds (for the model to be comparable to SB), and limited the number of training epochs to 200 (due to the validation loss stagnation, to prevent overfitting). Due to the fact that the Shifts dataset does not contain lesions less than 10 voxels, we process the outputs of each of the models to remove all the connected components with less than 10 voxels.

---

<sup>4</sup> The original code including model implementation and weights, training and inference code can be found at the Shifts Challenge GitHub: <https://github.com/Shifts-Project/shifts/tree/main/mswml>. nnU-Net model code is publicly available at <https://github.com/MIC-DKFZ/nnUNet>. Model weights can be found on our GitHub: [https://github.com/Medical-Image-Analysis-Laboratory/MS\\_WML\\_uncs](https://github.com/Medical-Image-Analysis-Laboratory/MS_WML_uncs).

### 3. Results

#### 3.1. Model performance

The evaluation of the ensemble model performance in terms of average segmentation and lesion detection quality is presented in Table 3 for training, validation, and testing sets. Regardless of the model, SB or nnU-Net, the in-domain performance reaches its upper bound determined by the inter-rater agreement reported in. There is a considerable drop in performance (around 10% depending on the metric) between in- and out-of-domain sets both in terms of segmentation (DSC and nDSC) and lesion detection (LF1). The performance on  $\text{Test}_{private}$  dataset lies in between  $\text{Test}_{in}$  and  $\text{Test}_{out}$  with regards to segmentation and lesion detection quality. Between two models, nnU-Net shows higher performance in terms of segmentation and lesion detection.

Set	DSC		nDSC		LF1		LPPV	
	SB	nnU-Net	SB	nnU-Net	SB	nnU-Net	SB	nnU-Net
Train	0.756 [0.737, 0.774]	0.906 [0.892, 0.917]	0.725 [0.699, 0.749]	0.856 [0.826, 0.883]	0.547 [0.493, 0.596]	0.845 [0.787, 0.876]	0.689 [0.627, 0.735]	0.971 [0.957, 0.981]
Val	0.720 [0.602, 0.783]	0.776 [0.701, 0.821]	0.684 [0.625, 0.740]	0.736 [0.669, 0.783]	0.444 [0.345, 0.547]	0.643 [0.555, 0.707]	0.533 [0.425, 0.608]	0.762 [0.624, 0.871]
$\text{Test}_{in}$	0.633 [0.582, 0.673]	0.707 [0.671, 0.739]	0.689 [0.662, 0.717]	0.741 [0.715, 0.768]	0.487 [0.439, 0.528]	0.701 [0.666, 0.733]	0.610 [0.552, 0.660]	0.762 [0.721, 0.797]
$\text{Test}_{out}$	0.488 [0.457, 0.515]	0.571 [0.538, 0.600]	0.533 [0.501, 0.560]	0.603 [0.570, 0.630]	0.333 [0.308, 0.361]	0.502 [0.477, 0.525]	0.623 [0.586, 0.659]	0.828 [0.799, 0.852]
$\text{Test}_{private}$	0.601 [0.578, 0.621]	0.646 [0.626, 0.665]	0.628 [0.608, 0.645]	0.653 [0.635, 0.670]	0.416 [0.396, 0.437]	0.562 [0.543, 0.581]	0.581 [0.556, 0.605]	0.799 [0.779, 0.817]

Table 3: Mean average models performance in segmentation (DSC and nDSC) and lesion detection (LF1 and LPPV). 90% confidence intervals were computed using bootstrapping. SB - Shifts 2.0 Challenge baseline model.

### 3.2. Quantitative evaluation of uncertainty measures

#### 3.2.1. Error retention curves analysis

The error RCs for the assessment of uncertainty measures on each of the anatomical scales (voxel, lesion, and patient) are presented in Figure 3. The voxel-scale DSC-RCs and lesion-scale LPPV-RCs were obtained by averaging across the respective datasets. The mean areas under the error retention curves and the results of the statistical testing are presented in Table 4.

Regardless of the test set, all **voxel-scale** uncertainty measures outperform random uncertainty and are closer to the ideal uncertainty in terms of mean DSC-AUC, indicating their ability to capture errors in segmentation. However, the marginal difference between DSC-AUCs of different measures is relatively small. On the in-domain  $\text{Test}_{in}$ , there is no agreement between two models in terms of the measures with the highest mean DSC-AUC: while total and data uncertainty ( $NC_i, EoE_i, ExE_i$ ) have higher DSC-AUC for the SB model, knowledge uncertainty ( $MI_i$ ) has a higher DSC-AUC for the nnU-Net model. On the out-of-domain  $\text{Test}_{out}$  and  $\text{Test}_{private}$  datasets, the entropy-based total and data uncertainty measures ( $EoE_i$  and  $ExE_i$ ) tend to have an advantage compared to other measures, contributing to their overall advantage in the whole evaluation. Nevertheless, the aggregation of data uncertainty  $ExE_i$  for the lesion-/ patient- uncertainty computation yields usually the worst results in terms of lesion-scale LPPV-AUC / patient-scale DSC-AUC. This means that a good performance of a uncertainty measure in capturing voxel misclassifications, when aggregated, will not necessarily lead to an optimal uncertainty measure to capture lesion false detection errors or overall segmentation failure.

Regardless of the test set, at the **lesion scale**, there is a greater marginal difference between different measures, particularly for the SB model. The proposed measure  $LSU^+$  often has an advantage in the mean LPPV-AUC over other measures, indicating a better ability to capture lesion false positive errors. While  $LSU$  and  $LSU^+$  have similar LPPV-AUCs, there is usually some difference in their performances, benefiting the  $LSU^+$  measure. Among the measures based on the aggregation of voxel uncertainties, aggregated total uncertainty  $\overline{EoE}_L$  generally provides slightly higher mean LPPV-AUC.

At the **patient scale**, the marginal differences between various measures are prominent compared to the voxel and lesion scales, especially on the out-

of-domain sets. The results are aligned for both in- and out-of-domain test sets and for both models, SB and nn-Unet. The proposed  $PSU^+$  and  $PSU$  measures have comparable and the highest patient-scale DSC-AUCs, suggesting their superior ability to capture overall segmentation failure. The aggregation of the best in terms of LPPV-AUC lesion scale uncertainty ( $LSU$ ) yields lower patient DSC-AUC. Averaging of voxel uncertainties across the brain generally provides worse-than-random performance in the error retention curve analysis. The last means that an average across-subject voxel-scale uncertainty is not informative of an overall segmentation performance on a particular subject measured by DSC, or has an inverse relationship with errors.

### 3.2.2. Patient-scale uncertainty as a proxy to the segmentation quality

Extending the analysis of the relationship between the patient-scale uncertainty measures and the segmentation quality measures by DSC, Table 5 presents corresponding Spearman's correlation coefficients. Figure 4 contains plots DSC and patient uncertainty for the measures with the highest (proposed  $PSU^{(+)}$ ), median (proposed  $\overline{LSU^+}$ ), and worse-than-random ( $\overline{NC}_B$  and  $\overline{EOE}_B$ ) patient-scale DSC-AUC values. For the SB model and for the rest of the measures, the same analysis and trends can be found in Appendix B. The results show the highest correlation between the patient uncertainty and DSC is provided by the proposed  $PSU^{(+)}$  measures, with  $\rho$  around 0.8 across different test sets. For the aggregation of the lesion-scale uncertainty the correlation with the segmentation quality drops at least twice, while for the measures based on the voxel-scale uncertainty aggregation, the correlation is either weak, e.g.  $\overline{NC}_B$ , or positive. There is a positive correlation between  $\overline{EOE}_B$ ,  $\overline{ExE}_B$ , and  $\overline{MI}_B$ , suggesting that high uncertainty can point to examples with high DSC. The absolute value of this correlation is around 0.5, which is higher than for  $\overline{LSU^{(+)}}$ , yet lower than for the proposed  $PSU^{(+)}$ .

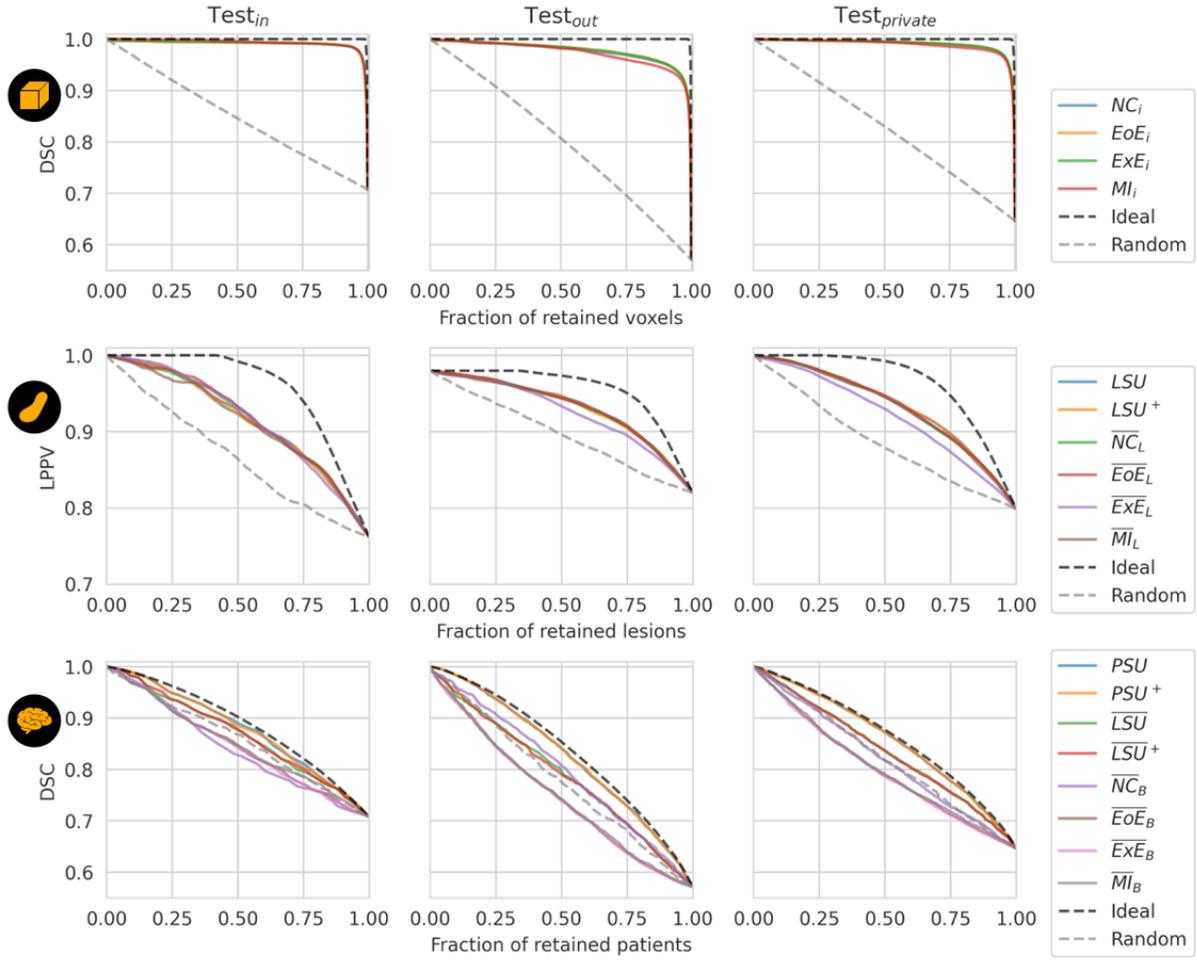


Figure 3: Error retention curves for the assessment of uncertainty measures at the voxel, lesion, and patient anatomical scales across the in-domain  $\text{Test}_{in}$  (left column) and the out-of-domain  $\text{Test}_{out}$  (center column) and  $\text{Test}_{private}$  (left column) sets for the nnU-Net model. Different rows correspond to different anatomical scales indicated with icons on the left. The voxel-scale DSC-RCs and lesion-scale LPPV-RCs were obtained by averaging across the respective datasets. At each of the scales, the ideal (black dashed) line indicates the upper bound of an uncertainty measure performance in its ability to capture model errors; the random (gray dashed) indicates no relationship between an uncertainty measure and error; a worse-than-random performance indicates an inverse relationship. Analogous results for the SB model are shown in Appendix B.1.

Measure	Test <sub>in</sub>		Test <sub>out</sub>		Test <sub>private</sub>	
	SB	nnU-Net	SB	nnU-Net	SB	nnU-Net
Voxel-scale DSC-AUC (↑)						
Ideal	99.93[99.91, 99.94]	99.94[99.92, 99.95]	99.90[99.88, 99.91]	99.93[99.92, 99.94]	99.92[99.91, 99.92]	99.93[99.92, 99.94]
$NC_i$	<b>99.17[98.99, 99.31]</b>	99.17[98.29, 99.49]	96.74[96.23, 97.12]	97.59[97.02, 0.9797]	98.56[98.36, 98.70]	<b>99.02[98.82, 99.16]</b>
$EoE_i$	<b>99.16[98.99, 99.31]</b>	<i>99.11[98.10, 99.46]</i>	<b>97.02[96.56, 97.37]</b>	<b>97.72[97.22, 98.05]</b>	<b>98.65[98.46, 98.79]</b>	<b>99.02[98.82, 99.17]</b>
$ExE_i$	<b>99.16[98.99, 99.31]</b>	<i>99.11[98.09, 99.46]</i>	<b>97.02[96.56, 97.38]</b>	<b>97.71[97.21, 98.05]</b>	<b>98.65[98.46, 98.80]</b>	<b>99.02[98.82, 99.16]</b>
$MI_i$	<i>99.05[98.85, 99.21]</i>	<b>99.27[98.74, 99.50]</b>	<i>96.69[96.19, 97.08]</i>	<i>97.28[96.70, 97.68]</i>	<i>98.46[98.25, 98.62]</i>	<i>98.86[98.63, 99.01]</i>
Random	80.91[76.77, 83.36]	84.87[82.79, 86.69]	76.20[74.88, 77.36]	80.00[78.72, 81.21]	80.18[78.99, 81.19]	82.79[81.85, 83.62]
Lesion-scale LPPV-AUC (↑)						
Ideal	87.88[82.60, 90.91]	95.72[93.89, 96.88]	87.07[83.40, 89.46]	96.47[93.13, 97.66]	86.41[84.54, 87.93]	96.36[95.51, 96.96]
$LSU$	83.54[78.50, 87.04]	91.54[89.57, 93.15]	83.28[79.63, 85.91]	<b>94.06[90.87, 95.41]</b>	82.63[80.74, 84.28]	<b>93.29[92.15, 94.21]</b>
$LSU^+$	<b>83.90[78.83, 87.31]</b>	91.51[89.53, 93.12]	<b>83.89[80.27, 86.45]</b>	93.97[90.80, 95.33]	<b>82.70[80.83, 84.37]</b>	<b>93.29[92.15, 94.20]</b>
$\overline{NC}_L$	83.33[78.34, 86.77]	91.71[89.46, 93.32]	83.24[79.60, 85.86]	<b>94.06[90.84, 95.39]</b>	82.34[80.38, 84.04]	93.14[92.05, 94.05]
$\overline{EoE}_L$	83.38[78.41, 86.83]	<b>91.81[89.61, 93.39]</b>	83.26[79.63, 85.88]	<b>94.07[90.86, 95.40]</b>	82.28[80.30, 83.99]	93.22[92.11, 94.11]
$\overline{ExE}_L$	<i>81.73[76.70, 85.24]</i>	91.70[89.50, 93.27]	<i>81.55[77.88, 84.17]</i>	<i>93.41[90.32, 94.77]</i>	<i>78.74[76.68, 80.56]</i>	<i>91.99[90.77, 93.00]</i>
$\overline{MI}_L$	82.63[77.70, 86.03]	<i>91.37[89.22, 92.98]</i>	82.31[78.64, 85.00]	<b>94.06[90.86, 95.40]</b>	81.62[79.69, 83.34]	93.05[91.89, 93.96]
Random	76.69[71.57, 80.48]	86.65[83.96, 88.94]	76.35[72.71, 79.19]	90.59[87.65, 92.10]	73.97[71.91, 75.81]	88.61[87.18, 89.88]
Patient-scale DSC-AUC (↑)						
Ideal	85.74 [84.16, 87.52]	88.72 [87.22, 90.36]	79.21 [77.96, 80.52]	83.55 [82.30, 84.95]	84.48 [83.72, 85.26]	86.23 [85.56, 86.91]
$PSU$	<b>84.99 [83.16, 86.81]</b>	<b>87.90 [86.25, 89.73]</b>	<b>78.40 [77.11, 79.73]</b>	<b>82.68 [81.26, 84.18]</b>	<b>83.63 [82.79, 84.47]</b>	<b>85.73 [85.02, 86.46]</b>
$PSU^+$	<b>84.82 [82.97, 86.68]</b>	<b>87.84 [86.17, 89.70]</b>	<b>78.39 [77.10, 79.70]</b>	<b>82.70 [81.28, 84.20]</b>	<b>83.60 [82.75, 84.44]</b>	<b>85.75 [85.04, 86.47]</b>
$\overline{LSU}$	83.77 [81.99, 85.42]	86.80 [84.69, 88.84]	75.48 [74.55, 77.26]	79.05 [77.66, 81.22]	79.91 [80.02, 82.28]	83.55 [82.54, 84.44]
$\overline{LSU}^+$	83.13 [81.04, 84.88]	86.87 [84.80, 88.89]	75.28 [74.36, 77.08]	78.96 [77.53, 81.16]	79.91 [80.02, 82.28]	83.52 [82.51, 84.42]
$\overline{NC}_B$	80.70 [78.27, 82.42]	<i>84.13 [82.40, 85.57]</i>	74.82 [72.96, 76.57]	79.90 [77.85, 81.73]	79.79 [78.55, 80.90]	82.00 [80.84, 82.97]
$\overline{EoE}_B$	80.19 [76.20, 82.86]	84.71 [82.40, 86.80]	<i>71.60 [69.62, 73.32]</i>	75.04 [72.79, 76.84]	77.43 [75.81, 78.79]	79.98 [78.49, 81.19]
$\overline{ExE}_B$	<i>80.19 [76.20, 82.87]</i>	84.64 [82.34, 86.72]	<i>71.57 [69.53, 73.31]</i>	<i>74.94 [72.69, 76.72]</i>	<i>77.37 [75.74, 78.73]</i>	<i>79.83 [78.33, 81.04]</i>
$\overline{MI}_B$	80.28 [76.25, 83.02]	85.07 [82.69, 87.20]	71.70 [69.76, 73.39]	75.18 [72.93, 77.00]	77.60 [75.97, 78.97]	80.20 [78.72, 81.42]
Random	81.87 [79.09, 83.84]	85.73 [83.58, 87.62]	74.10 [72.53, 75.53]	78.03 [76.20, 79.60]	80.08 [78.85, 81.14]	82.26 [81.14, 83.23]

Table 4: Mean average areas under error retention curves and 90% bootstrap confidence intervals for the assessment of the uncertainty measures at the voxel, lesion, and patient anatomical scales across the in-domain Test<sub>in</sub> (left column) and the out-of-domain Test<sub>out</sub> (center column) and Test<sub>private</sub> (right column) sets. Results are presented for the Shifts Challenge Baseline (SB) and nnU-Net models. Highest AUC values for each dataset, model, and anatomical scale are highlighted in **bold**, lowest - in *italic*; ideal and random values are in gray colour and indicate the upper and lower bounds of performance, respectively.

Measures	Test <sub>in</sub>		Test <sub>out</sub>		Test <sub>private</sub>		Test <sub>in+out</sub>		Test <sub>in+out+private</sub>	
	SB	nnU-Net	SB	nnU-Net	SB	nnU-Net	SB	nnU-Net	SB	nnU-Net
$PSU$	<b>-0.81</b>	<b>-0.83</b>	<b>-0.81</b>	-0.73	<b>-0.84</b>	-0.89	<b>-0.83</b>	<b>-0.76</b>	<b>-0.68</b>	<b>-0.59</b>
$PSU^+$	-0.75	-0.81	-0.8	<b>-0.74</b>	<b>-0.84</b>	<b>-0.9</b>	-0.82	<b>-0.76</b>	<b>-0.68</b>	<b>-0.59</b>
$\overline{LSU}$	-0.45	-0.36	-0.26	-0.25	-0.37	-0.27	-0.37	-0.24	-0.3	-0.09
$\overline{LSU}^+$	-0.29	-0.37	-0.22	-0.22	-0.34	-0.26	-0.3	-0.23	-0.25	-0.07
$\overline{NC}_B$	0.36	0.36	-0.1	-0.1	0	0	-0.2	-0.2	-0.18	-0.19
$\overline{EoE}_B$	0.23	0.28	0.55	0.54	0.54	0.57	0.56	0.57	0.49	0.5
$\overline{ExE}_B$	0.23	0.3	0.55	0.56	0.56	0.61	0.57	0.58	0.5	0.51
$\overline{MI}_B$	0.2	0.15	0.53	0.52	0.49	0.5	0.55	0.54	0.46	0.47

Table 5. Spearman correlation coefficients quantifying the relationship between different patient-scale uncertainty values and segmentation quality measured by DSC for different test sets and their combinations. The highest correlation coefficients are highlighted in **bold**.

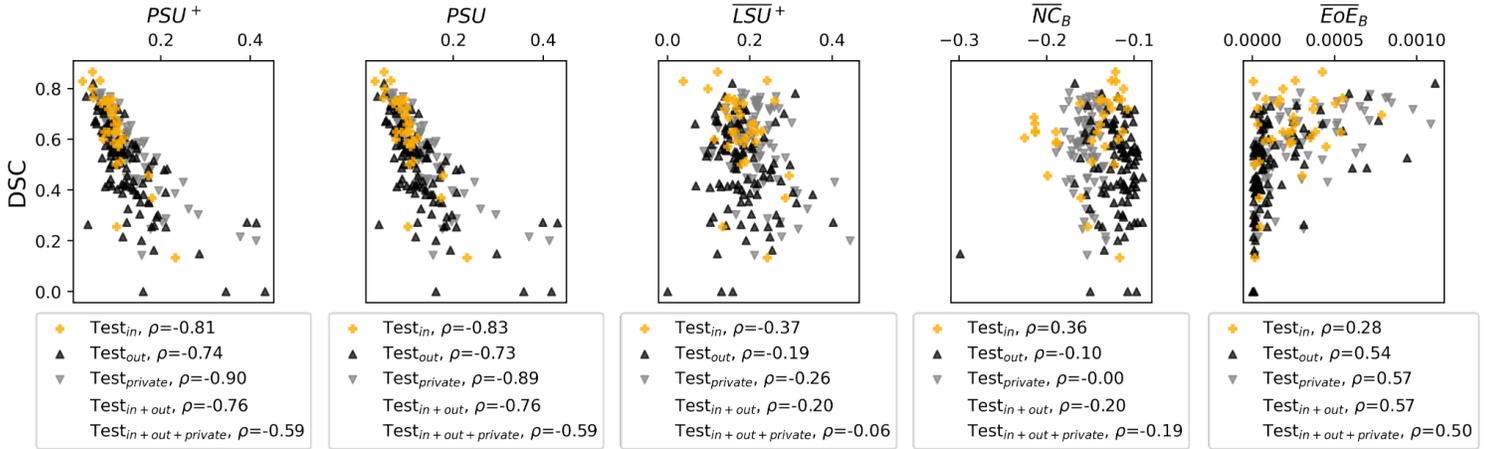


Figure 4: The relationship between DSC and patient-scale uncertainty assessed for  $Test_{in}$  (orange),  $Test_{out}$  (black),  $Test_{private}$  (gray) separately and jointly for the nnU-Net model. The presented uncertainty measures were chosen based on the results of the error RC analysis (Figure 3 and Table 4) to illustrate the relationship between DSC and uncertainty brought by measures with the highest (proposed  $PSU^+$ ), median (proposed  $\overline{LSU}^+$ ), and worse-than-random ( $\overline{NC}_B$  and  $\overline{EoE}_B$ ) DSC-AUC values. Analogous results for other measures and for the SB model can be seen in Appendix B.2.

### 3.3. Qualitative evaluation of the uncertainty maps

Our results show that uncertainty quantification mainly at the lesion and patient scales can well depict model error predictions, however, various anatomical scales provide information about different types of errors. In Figure 5 the uncertainty maps and values are shown for four different subjects, corresponding to different scenarios with respect to the quality of lesion segmentation.

**Voxel-scale maps** provide refined information about the misclassifications in each voxel. Moreover, voxel-scale uncertainty is always high at the borders of lesions. Hypothetically, this is a reflection of the inter-rater disagreement that introduces noise in the ground truth itself leading to further confusion / increased likelihood of having mistakes at the borders of lesions. Nevertheless, the voxel-scale uncertainty can be high in the center of the lesion, reflecting that the model is uncertain in the whole lesion region, not only at the borders. Sometimes high uncertainty regions can be related to the FNLs.

**Lesion-scale maps** provide a visually more intuitive way to assess the correctness of the predicted lesion regions compared to the voxel-scale maps. Particularly, lesion-scale maps can be used to highlight FPLs. Nonetheless, high lesion uncertainty may be an indicator of wrong delineation rather than detection. Let us note that, compared to the voxel-scale, the lesion-scale maps lose all the information about the FNLs.

**Patient-scale values** inform about the overall quality of the segmentation without indicating the particular reasons for the segmentation failure. As for the chosen examples (C) and (D), high patient uncertainty reveals the fact of the algorithm failure, however for (C) the problem is in the atypical large lesion and for (D) it is a wrong preprocessing, *i.e.* the absence of skull-stripping.

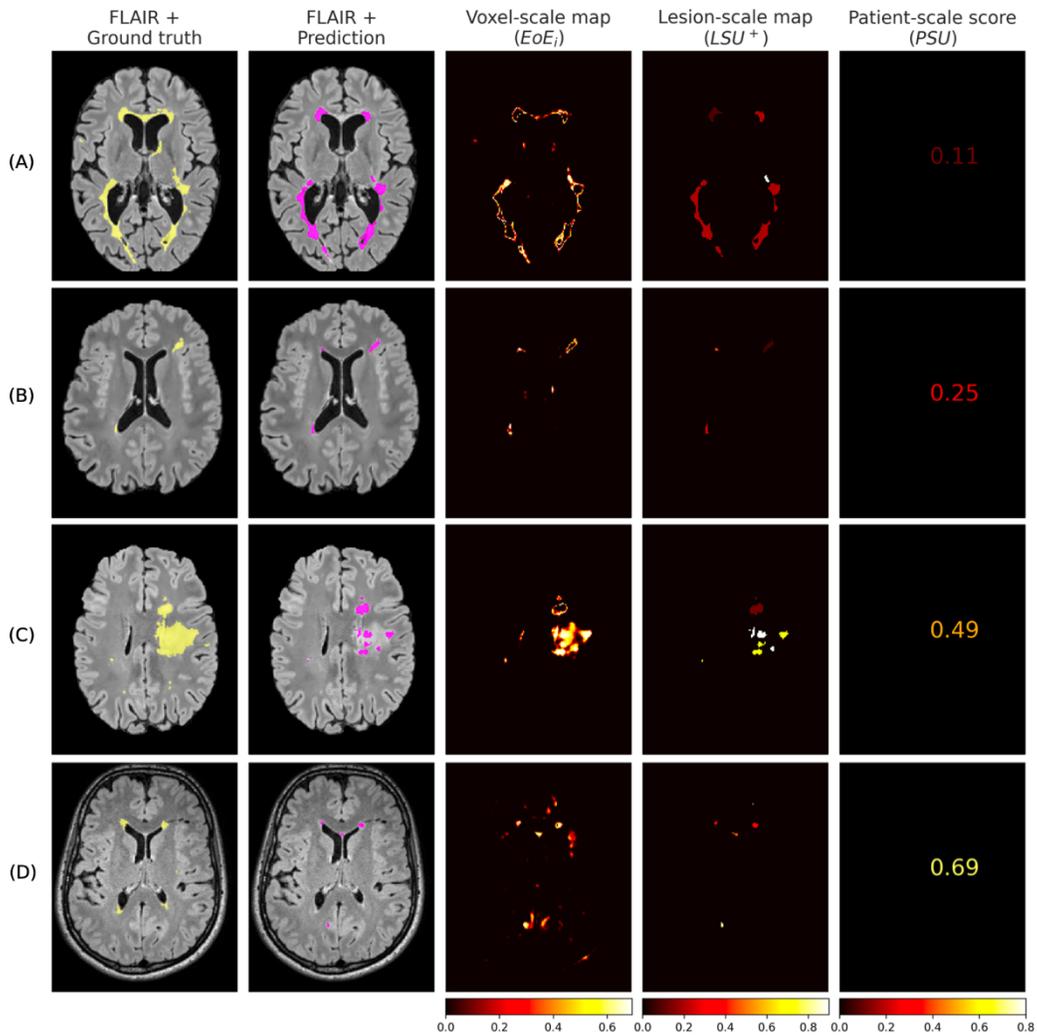


Figure 5: Examples of uncertainty maps at the voxel and lesion scales and patient uncertainty values. The two left columns illustrate axial slices of a FLAIR scan with the ground truth (in yellow) and predicted (in pink) WML masks; the middle column - voxel-scale uncertainty maps computed with the  $EoE_i$  measure; the fourth column - lesion-scale uncertainty maps computed with the proposed  $LSU^+$ ; the fifth column - the patient-scale uncertainty value computed with the proposed  $PSU^+$ . The choice of measures is based on the results of the error retention curves analysis. (A), (B), (C), and (D) represent different scenarios with gradually decreasing DSC. Cases (A) and (B) represent good and mediocre model performance, respectively. Patient (C) has an atypical large lesion, which the algorithm fails as expected. Patient (D) was not correctly preprocessed (the skull is not removed) which led to the algorithm's low performance and high patient uncertainty.

#### 4. Discussion

Our research offers a detailed framework for the assessment of uncertainty quantification for a clinically relevant task of white matter lesion segmentation in multiple sclerosis. The specificity of the segmentation task allowed for the exploration of UQ at different anatomical scales: voxel, lesion, and patient. We introduced novel structure-based UQ measures at the lesion and patient scales. On each of these scales, we performed a comparative study between different uncertainty measures (among the state-of-the-art and the proposed) to determine the measures that can point to the model errors of a particular kind: voxel misclassification, lesion false discovery, or overall low quality of segmentation. For this, we use the error retention curves analysis previously introduced for the pixel/ voxel scales (Malinin, 2019; Malinin et al., 2022; Mehta et al., 2022), and extended to the structural scales in this and our previous work (Molchanova et al., 2023). Our proposed uncertainty measures ( $LSU^{(+)}$  on the lesion scale and  $PSU^{(+)}$  on the patient scale from the equations 1-4) quantify the disagreement in the structural predictions between the ensemble model and its members, demonstrating enhanced error detection over state-of-the-art aggregation-based metrics on both in- and out-of-domain datasets. Furthermore,  $PSU^{(+)}$  is shown to be a reliable indicator of overall segmentation quality both in- and out-of-domain.

This study compares a variety of voxel-scale measurements adopted from classification tasks, noting their similar capabilities in capturing voxel misclassification errors. A more pronounced difference between these measures is observed after aggregation at other anatomical scales. Particularly, at the lesion scale, higher areas under the respective RCs are observed for the total uncertainty measures, compared to the measure of knowledge uncertainty, and even more data uncertainty. However, voxel uncertainty aggregation at the patient scale yielded results akin to random uncertainty judging by the error RC analysis. Closer examination of the correlation between patient scale uncertainty measures and the DSC revealed a positive relationship, suggesting that a higher average voxel uncertainty correlates with improved DSC. To explain this counterintuitive finding, we need to recall the fact that the model is biased towards segmenting better subjects with higher lesion load which comes from the loss

function construction and has been previously highlighted in (Raina et al., 2023).

Then, considering our qualitative assessment revealing that the uncertainty is the highest at the borders of lesions, the positive correlation between average voxel uncertainty in a subject and the DSC on this subject becomes clear. Similar behaviour of the measures based on an aggregation of voxel uncertainties has been previously observed for the task of brain tumor segmentation (Jungo et al., 2020), but not for the task of brain structures segmentation (Roy et al., 2019), where the segmented objects are the same and of similar sizes in each of the images. This supports our hypothesis that voxel-scale uncertainty aggregation is unsuitable for tasks affected by this bias. In such cases, structural disagreement metrics present a viable alternative to aggregation-based methods, showing a strong connection to different error types.

#### *4.1 Limitations and future work*

The fact that lesion and patient uncertainty measures depend on the choice of the threshold at the model's output, necessary for the instances / segmented region definition, remains a matter of ongoing debate. We proposed to address the issue by introducing two analogs of the same measure corresponding to different strategies of the threshold choice, i.e.  $LSU$  versus  $LSU^+$  and  $PSU$  and  $PSU^+$ . Nevertheless, a more detailed investigation of this aspect might be needed. For instance, exploring the model calibration as a way to circumvent threshold tuning or investigating measures of uncertainty where this dependence is mitigated.

This paper is focused on the WML segmentation task. While this is a very relevant task in clinical practice, there are several medical image segmentation tasks that could adopt the proposed multi-scale approach for UQ. This includes, for instance, nuclei segmentation on histopathology images (Kumar et al., 2020), bone metastases segmentation on the full-body MRI or CT (Colombo et al., 2021; Afnouch et al., 2023), vascularized lymph nodes on CT or MRI (Hassani et al., 2020), or white matter lesions in MRI from non-MS patients (Malova et al., 2021). Still, finding the multi-centric data and benchmarks needed for UQ methods validation under the domain shift in these new tasks is not straightforward.

While Trustworthy AI gains momentum, the practical integration of uncertainty measures in clinical workflows necessitates further investigation and clinical feedback, balancing the provision of additional information to clinicians with the risk of biasing their decisions poses a unique challenge (Evans et al., 2022b). Given the knowledge about the information brought by uncertainty quantified at different scales and the relationship of uncertainty to errors, it is further important to investigate different transitional scenarios and the potential perceptual biases that the uncertainty (maps) can create in the perception of clinicians. Thus, future research direction should focus on obtaining clinical feedback to study the perception, usability, and biases induced by showing uncertainty maps to radiologists. It would be particularly important to pursue a clinical validation of the hypotheses made about the informativeness of the proposed measures as a way to point clinicians to model errors.

## **Acknowledgments**

This work was supported by the Hasler Foundation Responsible AI programme (MSxplain), the EU Horizon 2020 project AI4Media (grant 951911), and the Swiss National Science Foundation (SNF) Postdoc Mobility Fellowship (P500PB\_206833). We acknowledge access to the facilities and expertise of the CIBM Center for Biomedical Imaging, a Swiss research center of excellence founded and supported by Lausanne University Hospital (CHUV), University of Lausanne (UNIL), École polytechnique fédérale de Lausanne (EPFL), University of Geneva (UNIGE) and Geneva University Hospitals (HUG). This research is partially funded by the EPSRC (The Engineering and Physical Sciences Research Council) Doctoral Training Partnership (DTP) PhD studentship and supported by Cambridge University Press & Assessment (CUP&A), a department of The Chancellor, Masters, and Scholars of the University of Cambridge.

## **Declaration of Generative AI Usage and AI-assisted technologies**

During the preparation of this work the authors used ChatGPT-3.5/-4 and Grammarly for the detection of grammatic and stylistic errors in the manuscript. After using these tools, the authors reviewed and edited the content as needed and take full responsibility for the content of the publication.

## Appendix A. Definitions of quality metrics

Let  $\#_{TP}, \#_{FP}, \#_{FN}$  be the number of true positive (TP), false positive (FP), and false negative (FN) voxels, respectively.

$$\text{True positive rate: } TPR = \frac{\#_{TP}}{\#_{TP} + \#_{FN}}.$$

$$\text{Positive predictive value: } PPV = \frac{\#_{TP}}{\#_{TP} + \#_{FP}}.$$

$$\text{Dice similarity score or } F_1\text{-score: } DSC = F_1 = \frac{TPR \cdot PPV}{TPR + PPV} = \frac{2 \cdot \#_{TP}}{2 \cdot \#_{TP} + \#_{FP} + \#_{FN}}.$$

**Normalized Dice similarity score** Raina et al. (2023):

$$nDSC = \frac{2 \cdot \#_{TP}}{2 \cdot \#_{TP} + \kappa \cdot \#_{FP} + \#_{FN}}, \kappa = h(r^{-1} - 1),$$

where  $h$  represents the ratio between the positive and the negative classes while  $0 < r < 1$  denotes a *reference* value that is set to the mean fraction of the positive class, *i.e.* a lesion class in our case, across a large number of subjects.

Analogous, lesion-scale metrics can be defined by replacing  $\#_{TP}, \#_{FP}, \#_{FN}$  with a number of TP, FP, and FN lesions (TPL, FPL, FNL). As mentioned before, the definition of lesion types can vary. This work uses 25% overlap to distinguish TPL and FPL among the predicted lesions. FNL is defined as the ground truth lesions that have no overlap with predictions.

## Appendix B. Additional results

### B.1 Error retention curve analysis

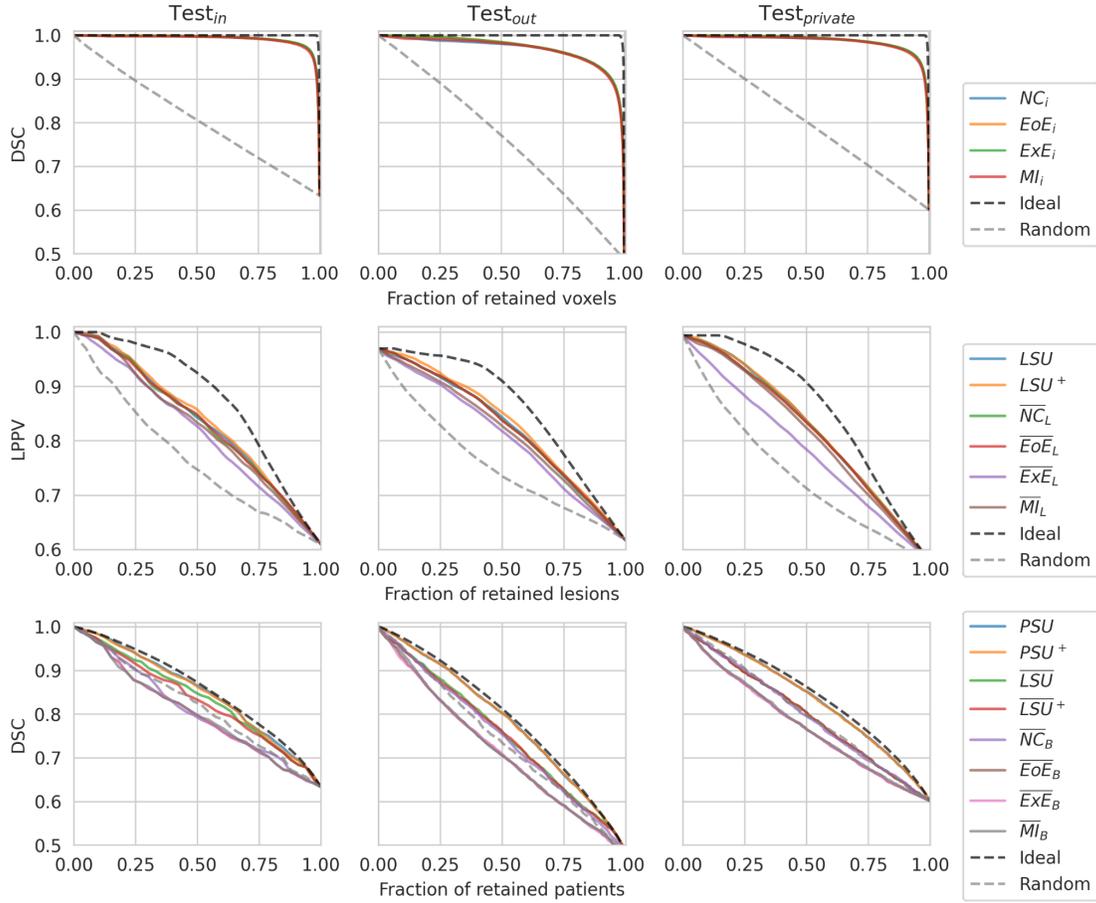


Figure 6: Error retention curves for the assessment of uncertainty measures at the voxel, lesion, and patient (rows one, two, and three, respectively) anatomical scales across the in-domain  $Test_{in}$  (left column) and the out-of-domain  $Test_{out}$  (center column) and  $Test_{private}$  (right column) sets for the SB model. Different rows correspond to different anatomical scales indicated with icons on the left. The voxel-scale DSC-RCs and lesion-scale LPPV-RCs were obtained by averaging across the respective datasets. At each of the scales, the ideal (black dashed) line indicates the upper bound of an uncertainty measure performance in its ability to capture model errors; the random (gray dashed) indicates no relationship between an uncertainty measure and error; a worse-than-random performance indicates an inverse relationship.

## B.2 Patient-scale uncertainty as a proxy for segmentation quality

Figures 7 and 8 extend the error retention curves analysis of the patient-scale uncertainty measures revealing more information about the relationship between the uncertainty measures and the segmentation quality measures by DSC.

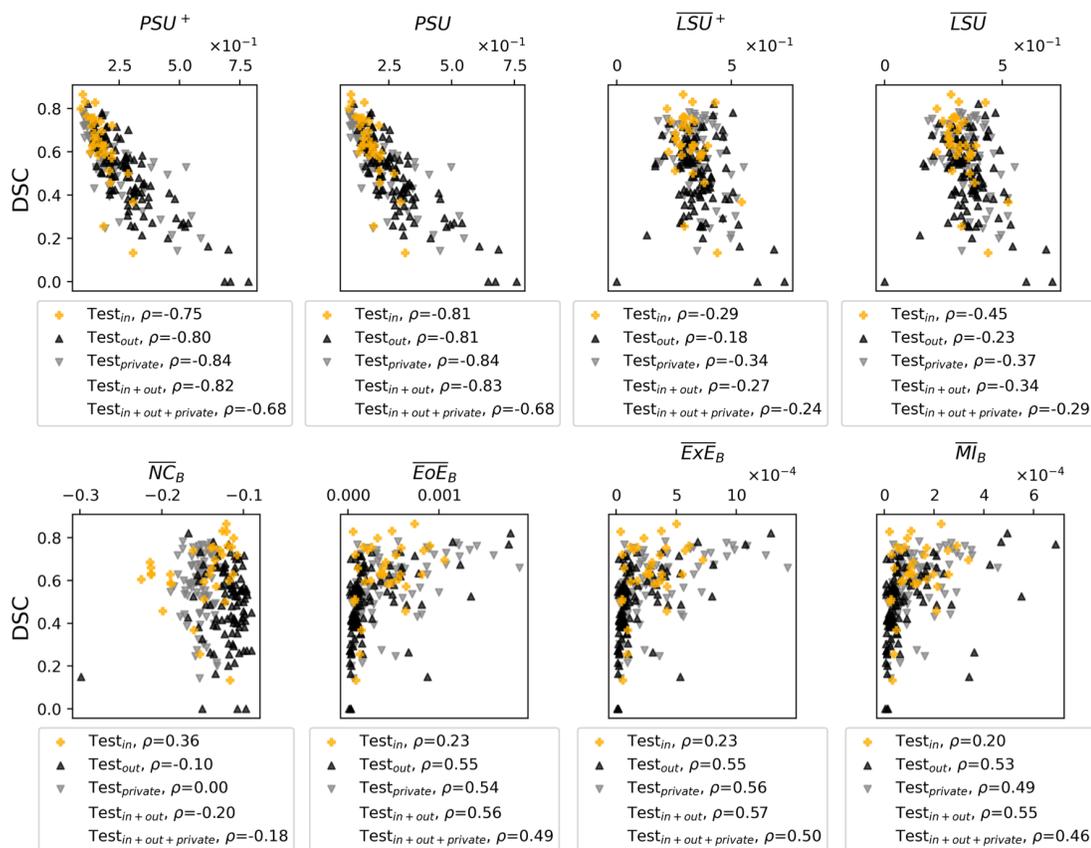


Figure 7: The relationship between DSC and patient-scale uncertainty assessed for  $Test_{in}$  (orange),  $Test_{out}$  (black), and  $Test_{private}$  (gray) separately and jointly for the SB model. The Spearman correlation coefficients  $\rho$  between DSC and uncertainty are reported in the plots' legends.

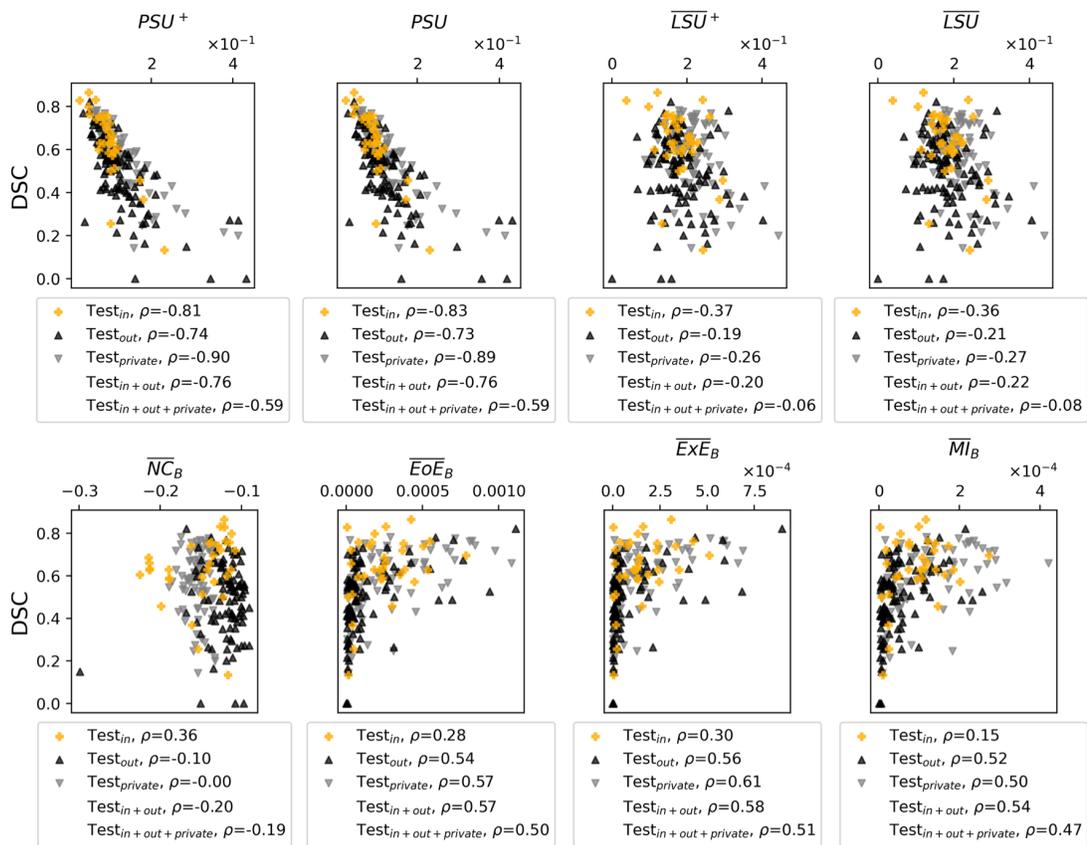


Figure 8: The relationship between DSC and patient-scale uncertainty assessed for  $Test_{in}$  (orange),  $Test_{out}$  (black), and  $Test_{private}$  (gray) separately and jointly for the nnU-Net model. The Spearman correlation coefficients  $\rho$  between DSC and uncertainty are reported in the plots' legends.

## References

- Afnouch, M., Gaddour, O., Hentati, Y., Bougourzi, F., Mohamed, A., Alouani, I., & Ahmed, A. T. (2023). BM-Seg: A new bone metastases segmentation dataset and ensemble of CNN-based segmentation approach. *Expert Systems With Applications*, 228, 120376.
- Begoli, E., Bhattacharya, T., and Kusnezov, D. F. (2019). The need for uncertainty quantification in machine-assisted medical decision making. *Nature Machine Intelligence*, 1(1).
- [dataset] Bonnier, G., Roche, A., Romascano, D., Simioni, S., Meskaldji, D., Rotzinger, D., Lin, Y.-C., Menegaz, G., Schlupe, M., Du Pasquier, R., Sumpf, T. J., Frahm, J., Thiran, J.-P., Krueger, G., and Granziera, C. (2014). Advanced mri unravels the nature of tissue alterations in early multiple sclerosis. *Annals of Clinical and Translational Neurology*, 1(6):423–432.
- [dataset] Carass, A., Roy, S., Jog, A., Cuzzocreo, J. L., Magrath, E., Gherman, A., Button, J., Nguyen, J., Prados, F., Sudre, C. H., Jorge Cardoso, M., Cawley, N., Ciccarelli, O., Wheeler-Kingshott, C. A., Ourselin, S., Catanese, L., Deshpande, H., Maurel, P., Commowick, O., Barillot, C., Tomas-Fernandez, X., Warfield, S. K., Vaidya, S., Chunduru, A., Muthuganapathy, R., Krishnamurthi, G., Jesson, A., Arbel, T., Maier, O., Handels, H., IHEME, L. O., Unay, D., Jain, S., Sima, D. M., Smeets, D., Ghafoorian, M., Platel, B., Birenbaum, A., Greenspan, H., Bazin, P.L., Calabresi, P. A., Crainiceanu, C. M., Ellingsen, L. M., Reich, D. S., Prince, J. L., and Pham, D. L. (2017). Longitudinal multiple sclerosis lesion segmentation: Resource and challenge. *NeuroImage*, 148:77–102.
- [dataset] Commowick, O., Istace, A., Kain, M., Laurent, B., Leray, F., Simon, M., Pop, S., Girard, P., Ameli, R., Ferré, J.-C., Kerbrat, A., Tourdias, T., Cervenansky, F., Glatard, T., Beaumont, J., Doyle, S., Forbes, F., Knight, J., Khademi, A., and Barillot, C. (2018). Objective evaluation of multiple sclerosis lesion segmentation using a data management and processing infrastructure. *Scientific Reports*, 8:13650–13666.

- Çiçek, Ö., Abdulkadir, A., Lienkamp, S. S., Brox, T., & Ronneberger, O. (2016). 3D U-Net: Learning Dense Volumetric Segmentation from Sparse Annotation. In Lecture notes in computer science (pp. 424–432).
- Colombo, A., Saia, G., Azzena, A. A., Rossi, A., Zugni, F., Pricolo, P., Summers, P., Marvaso, G., Grimm, R., Bellomi, M., Jereczek-Fossa, B. A., Padhani, A. R., & Petralia, G. (2021). Semi-Automated Segmentation of Bone Metastases from Whole-Body MRI: Reproducibility of Apparent Diffusion Coefficient Measurements. *Diagnostics*, 11(3), 499.
- Coupé, P., Yger, P., Prima, S., Hellier, P., Kervrann, C., and Barillot, C. (2008). An optimized blockwise nonlocal means denoising filter for 3-d magnetic resonance images. *IEEE Transactions on Medical Imaging*, 27.
- Faghani, S., Moassefi, M., Rouzrokh, P., Khosravi, B., Baffour, F. I., Ringler, M. D., and Erickson, B. J. (2023). Quantifying uncertainty in deep learning of radiologic images. *Radiology*, 308(2):e222217. PMID: 37526541.
- Fartaria, M. J., Kober, T., Granziera, C., and Bach Cuadra, M. (2019). Longitudinal analysis of white matter and cortical lesions in multiple sclerosis. *NeuroImage: Clinical*, 23:101938.
- Fartaria, M. J., Todea, A., Kober, T., O'brien, K., Krueger, G., Meuli, R., Granziera, C., Roche, A., and Bach Cuadra, M. (2018). Partial volume-aware assessment of multiple sclerosis lesions. *NeuroImage: Clinical*, 18:245–253.
- Gal, Y. (2016). *Uncertainty in Deep Learning*. PhD thesis, University of Cambridge, United Kingdom.
- Gal, Y. and Ghahramani, Z. (2015). Dropout as a bayesian approximation: Representing model uncertainty in deep learning. *Proceedings of The 33rd International Conference on Machine Learning*.
- Gawlikowski, J., Tassi, C., Ali, M., Lee, J., Humt, M., Feng, J., Kruspe, A., Triebel, R., Jung, P., Roscher, R., Shahzad, M., Yang, W., Bamler, R., and Zhu, X. (2023). A survey of uncertainty in deep neural networks. *Artificial Intelligence Review*, pages 1–77.

- Gramsch, C., Nensa, F., Kastrup, O., Maderwald, S., Deuschl, C., Ringelstein, A., Schelhorn, J., Forsting, M., and Schlamann, M. (2015). Diagnostic value of 3D fluid attenuated inversion recovery sequence in multiple sclerosis. *Acta Radiologica*, 56(5):622–627.
- Graziani, M., Dutkiewicz, L., Calvaresi, D., Amorim, J. P., Yordanova, K., Vered, M., Nair, R., Abreu, P. H., Blanke, T., Pulignano, V., Prior, J. O., Lauwaert, L., Reijers, W., Depeursinge, A., Andrearczyk, V., & Müller, H. (2022). A global taxonomy of interpretable AI: unifying the terminology for the technical and social sciences. *Artificial Intelligence Review*, 56(4), 3473–3504.
- Hassani, C., Tran, K., Palmer, S., & Patel, K. M. (2020). Vascularized lymph node transfer: a primer for the radiologist. *Radiographics*, 40(4), 1073–1089.
- Hemond, C. and Bakshi, R. (2018). Magnetic resonance imaging in multiple sclerosis. *Cold Spring Harbor Perspectives in Medicine*, 8(5).
- [dataset] Granziera, C. (2018) Imaging the Interplay Between Axonal Damage and Repair in Multiple Sclerosis (INsIDER). <https://classic.clinicaltrials.gov/ct2/show/NCT05177523>.
- Isensee, F., Schell, M., Pflueger, I., Brugnara, G., Bonekamp, D., Neuberger, U., Wick, A., Schlemmer, H.-P., Heiland, S., Wick, W., Bendszus, M., Maier-Hein, K., and Kickingereider, P. (2019). Automated brain extraction of multisequence mri using artificial neural networks. *Human Brain Mapping*, 40.
- Isensee, F., Jaeger, P. F., Kohl, S., Petersen, J., & Maier-Hein, K. H. (2020). nnU-Net: a self-configuring method for deep learning-based biomedical image segmentation. *Nature Methods*, 18(2), 203–211.
- Jungo, A., Balsiger, F., and Reyes, M. (2020). Analyzing the quality and challenges of uncertainty estimations for brain tumor segmentation. *Frontiers in Neuroscience*, 14.

- Kaur, A., Kaur, L., and Singh, A. (2020). State-of-the-art segmentation techniques and future directions for multiple sclerosis brain lesions. *Archives of Computational Methods in Engineering*, 28:1–27.
- Kumar, N., Verma, R., Anand, D., Zhou, Y., Onder, O. F., Tsougenis, E., Chen, H., Heng, P., Li, J., Hu, Z., Wang, Y., Koohbanani, N. A., Jahanifar, M., Tajeddin, N. Z., Gooya, A., Rajpoot, N., Ren, X., Zhou, S., Wang, Q., . . . Sethi, A. (2020). A Multi-Organ nucleus segmentation challenge. *IEEE Transactions on Medical Imaging*, 39(5), 1380–1391.
- La Rosa, F., Abdulkadir, A., Fartaria, M. J., Rahmanzadeh, R., Lu, P.-J., Galbusera, R., Baraković, M., Thiran, J., Granziera, C., and Cuadra, M. B. (2020). Multiple sclerosis cortical and WM lesion segmentation at 3T MRI: a deep learning method based on FLAIR and MP2RAGE. *NeuroImage: Clinical*, 27:102335.
- Lakshminarayanan, B., Pritzel, A., and Blundell, C. (2017). Simple and scalable predictive uncertainty estimation using deep ensembles. In Guyon, I., Luxburg, U. V., Bengio, S., Wallach, H., Fergus, R., Vishwanathan, S., and Garnett, R., editors, *Advances in Neural Information Processing Systems*, volume 30, pages 1–12. Curran Associates, Inc.
- Lambert, B., Forbes, F., Doyle, S., Tucholka, A., and Dojat, M. (2022a). Beyond voxel prediction uncertainty: Identifying brain lesions you can trust. *International Workshop on Interpretability of Machine Intelligence in Medical Image Computing*, pages 61–70.
- Lambert, B., Forbes, F., Doyle, S., Tucholka, A., and Dojat, M. (2022b). Fast Uncertainty Quantification for Deep Learning-based MR Brain Segmentation. In *EGC 2022 - Conference francophone pour l'Extraction et la Gestion des Connaissances*, pages 1–12, Blois, France.
- Lambert, B., Forbes, F., Tucholka, A., Doyle, S., Dehaene, H., and Dojat, M. (2022c). Trustworthy clinical ai solutions: a unified review of uncertainty quantification in deep learning models for medical image analysis. Preprint.

- [dataset] Lesjak, Z., Galimzianova, A., Koren, A., Lukin, M., Pernus, F., Likar, B., and Ziga piclin (2017). A novel public mr image dataset of multiple sclerosis patients with lesion segmentations based on multi-rater consensus. *Neuroinformatics*, 16:51–63.
- Lladó, X., Oliver, A., Cabezas, M., Freixenet, J., Vilanova, J. C., Quiles, A., Valls, L., Ramió-Torrentà, L., and Rovira, A. (2012). Segmentation of multiple sclerosis lesions in brain mri: A review of automated approaches. *Information Sciences*, 186(1):164–185.
- Malinin, A. (2019). *Uncertainty estimation in deep learning with application to spoken language assessment*. PhD thesis, University of Cambridge, United Kingdom.
- [dataset] Malinin, A., Athanasopoulos, A., Barakovic, M., Bach Cuadra, M., Gales, M. J. F., Granziera, C., Graziani, M., Kartashev, N., Kyriakopoulos, K., Lu, P.-J., Molchanova, N., Nikitakis, A., Raina, V., Rosa, F. L., Sivena, E., Tsarsitalidis, V., Tsompopoulou, E., and Volf, E. (2022). Shifts 2.0: Extending the dataset of real distributional shifts.
- Malova, M., Morelli, E., Cardiello, V., Tortora, D., Severino, M., Calevo, M. G., Parodi, A., De Angelis, L., Minghetti, D., Rossi, A., & Ramenghi, L. A. (2021). Nosological differences in the nature of punctate white matter lesions in preterm infants. *Frontiers in Neurology*, 12.
- McKinley, R., Wepfer, R., Grunder, L., Aschwanden, F., Fischer, T., Friedli, C., Muri, R., Rummel, C., Verma, R., Weisstanner, C., Wiestler, B., Berger, C., Eichinger, P., Mühlau, M., Reyes, M., Salmen, A., Chan, A. T., Wiest, R., and Wagner, F. (2020). Automatic detection of lesion load change in Multiple Sclerosis using convolutional neural networks with segmentation confidence. *NeuroImage: Clinical*, 25:102104.
- Mehta, R., Filo, A., Baid, U., Sako, C., McKinley, R., Rebsamen, M., Da'wyler, K., Meier, R., Radojewski, P., Murugesan, G. K., Nalawade, S. S., Ganesh, C., Wagner, B., Yu, F., Fei, B., Madhuranthakam, A. J., Maldjian, J. A., Daza, L., Gómez, C., Arbeláez, P., Dai, C., Wang, S., Reynaud, H., Mo, Y., Angelini, E. D., Guo, Y., Bai, W., Banerjee, S., Pei, L., Ak, M., Rosas-González, S., Zemmoura, I., Tauber, C., Vu, M. H., Nyholm, T., L'ofstedt, T., Ballestar, L.

M., Vilaplana, V., McHugh, H., Talou, G. D. M., Wang, A., Patel, J., Chang, K., Hoebel, K., Gidwani, M., Arun, N., Gupta, S., Aggarwal, M., Singh, P., Gerstner, E. R., Kalpathy-Cramer, J., Boutry, N., Huard, A., Vidyaratne, L., Rahman, M. M., Iftekharuddin, K. M., Chazalon, J., Puybureau, E., Tochon, G., Ma, J., Cabezas, M., Lladó, X., Oliver, A., Valencia, L., Valverde, S., Amian, M., Soltaninejad, M., Myronenko, A., Hatamizadeh, A., Feng, X., Quan, D., Tustison, N. J., Meyer, C. H., Shah, N., Talbar, S. N., Weber, M., Mahajan, A., Jakab, A., Wiest, R., Fathallah-Shaykh, H. M., Nazeri, A., Milchenko, M., Marcus, D. S., Kotrotsou, A., Colen, R. R., Freymann, J., Kirby, J., Davatzikos, C., Menze, B. H., Bakas, S., Gal, Y., and Arbel, T. (2022). QU-BRATS: MICCAI BRATS 2020 Challenge on Quantifying Uncertainty in Brain Tumor segmentation – Analysis of ranking scores and benchmarking results. *The Journal of Machine Learning for Biomedical Imaging*, 1(August 2022):1–54.

Molchanova, N., Raina, V., Malinin, A., La Rosa, F., Müller, H., Gales, M., Granziera, C., Graziani, M., and Bach Cuadra, M. (2023). Novel structural-scale uncertainty measures and error retention curves: Application to multiple sclerosis. In *2023 IEEE 20th International Symposium on Biomedical Imaging (ISBI)*, pages 1–5.

Nair, T., Precup, D., Arnold, D., and Arbel, T. (2020). Exploring uncertainty measures in deep networks for multiple sclerosis lesion detection and segmentation. *Medical Image Analysis*, 59:101557.

Raina, V., Molchanova, N., Graziani, M., Malinin, A., Muller, H., Bach Cuadra, M., and Gales, M. (2023). Novel structural-scale uncertainty measures and error retention curves: Application to multiple sclerosis. In *2023 IEEE 20th International Symposium on Biomedical Imaging (ISBI)*, pages 1–5.

Reich, D., Lucchinetti, C., and Calabresi, P. (2018). Multiple Sclerosis. *New England Journal of Medicine*, 378(2):169–180.

Reyes, M., Meier, R., Pereira, S., Silva, C. A., Dahlweid, F.-M., TenggKobligk, H. v., Summers, R. M., and Wiest, R. (2020). On the interpretability of artificial intelligence in radiology: Challenges and opportunities. *Radiology: Artificial Intelligence*, 2(3):e190043. PMID: 32510054.

- Ronneberger, O., Fischer, P., & Brox, T. (2015). U-NET: Convolutional Networks for Biomedical Image Segmentation. In Lecture notes in computer science (pp. 234–241).
- Rottmann, M., Colling, P., Hack, T.-P., Chan, R., Hüger, F., Schlicht, P., and Gottschalk, H. (2019). Prediction error meta classification in semantic segmentation: Detection via aggregated dispersion measures of softmax probabilities.
- Roy, A. G., Conjeti, S., Navab, N., and Wachinger, C. (2019). Bayesian quicknat: Model uncertainty in deep whole-brain segmentation for structurewise quality control. *NeuroImage*, 195:11–22.
- Spagnolo, F., Depeursinge, A., Schädelin, S., Akbulut, A., Müller, H., Barakovic, M., Melie-Garcia, L., Bach Cuadra, M., and Granziera, C. (2023). How far ms lesion detection and segmentation are integrated into the clinical workflow? a systematic review. *NeuroImage: Clinical*, 39:103491.
- Thompson, A. J., Banwell, B., Barkhof, F., Carroll, W. M., Coetsee, T., Comi, G., Correale, J., Fazekas, F., Filippi, M., Freedman, M. S., Fujihara, K., Galetta, S., Hartung, H. P., Kappos, L., Lublin, F., Marrie, R. A., Miller, A., Miller, D. H., Montalbán, X., Mowry, E. M., Sørensen, P. S., Tintoré, M., Traboulsee, A., Trojano, M., Uitdehaag, B. M. J., Vukusic, S., Waubant, E., Weinshenker, B. G., Reingold, S. C., and Cohen, J. A. (2018). Diagnosis of multiple sclerosis: 2017 revisions of the McDonald criteria. *Lancet Neurology*, 17(2):162–173.
- Tustison, N. J., Avants, B. B., Cook, P. A., Zheng, Y., Egan, A., Yushkevich, P. A., and Gee, J. C. (2010). N4itk: Improved n3 bias correction. *IEEE Transactions on Medical Imaging*, 29(6):1310–1320.
- Walton, C., King, R., Rechtman, L., Kaye, W., Leray, E., Marrie, R. A., Robertson, N., Rocca, N. L., Uitdehaag, B., van der Mei, I., Wallin, M., Helme, A., Napier, C. A., Rijke, N., and Baneke, P. (2020). Rising prevalence of multiple sclerosis worldwide: Insights from the atlas of ms, third edition. *Multiple Sclerosis Journal*, 26(14):1816–1821. PMID: 33174475.

- Wang, G., Li, W., Ourselin, S., and Vercauteren, T. (2019). Automatic brain tumor segmentation based on cascaded convolutional neural networks with uncertainty estimation. *Frontiers in Computational Neuroscience*, 13.
- Wattjes, M. P., Ciccarelli, O., Reich, D. S., Banwell, B., De Stefano, N., Enzinger, C., Fazekas, F., Filippi, M., Frederiksen, J. L., Gasperini, C., Hacoheh, Y., Kappos, L., Li, D. K., Mankad, K., Montalbán, X., Newsome, S. D., Oh, J., Palace, J., Rocca, M., Sastre-Garriga, J., Tintore, M., Vrenken, H., Yousry, T., Barkhof, F., and Rovira, À. (2021). 2021 MAGNIMS–CMSC–NAIMS consensus recommendations on the use of MRI in patients with multiple sclerosis. *Lancet Neurology*, 20(8), 653–670. [https://doi.org/10.1016/s1474-4422\(21\)00095-8](https://doi.org/10.1016/s1474-4422(21)00095-8)
- Whitbread, L. and Jenkinson, M. (2022). Uncertainty categories in medical image segmentation: A study of source-related diversity. In *Uncertainty for Safe Utilization of Machine Learning in Medical Imaging*, pages 26–35. Springer Nature Switzerland.
- Zeng, C., Gu, L., Liu, Z., and Zhao, S. (2020). Review of deep learning approaches for the segmentation of multiple sclerosis lesions on brain mri. *Frontiers in Neuroinformatics*, 14.
- Zou, K., Chen, Z., Yuan, X., Shen, X., Wang, M., and Fu, H. (2023). A review of uncertainty estimation and its application in medical imaging. *Meta-Radiology*, 1(1):100003.