
Repetitive Motion Estimation Network: Recover cardiac and respiratory signal from thoracic imaging

Xiaoxiao Li
Yale University

Vivek Singh
Siemens Medical Solutions USA Inc.

Yifan Wu
Siemens Medical Solutions USA Inc.

Klaus Kirchberg
Siemens Medical Solutions USA Inc.

James Duncan
Yale University

Ankur Kapoor
Siemens Medical Solutions USA Inc.

Abstract

Tracking organ motion is important in image-guided interventions, but motion annotations are not always easily available. Thus, we propose Repetitive Motion Estimation Network (RMEN) to recover cardiac and respiratory signals. It learns the spatio-temporal repetition patterns, embedding high dimensional motion manifolds to 1D vectors with partial motion phase boundary annotations. Compared with the best alternative models, our proposed RMEN significantly decreased the QRS peaks detection offsets by 59.3%. Results showed that RMEN could handle the irregular cardiac and respiratory motion cases. Repetitive motion patterns learned by RMEN were visualized and indicated in the feature maps.¹

1 Introduction

Cardiac interventions are often performed under the guidance of projective X-ray imaging on a beating heart. In such cardiac image-guided interventions, the organ motion can cause artifacts in the acquired images and lead to misalignment between the static guidance information that is overlaid on these images to guide the physician[1]. Studies to recover the organ motion signal directly from imaging by estimating explicit motion models [2, 3] have shown that specialized motion monitors or implanted markers are not necessary for accurate motion recovery. Recently, deep learning has been well-developed for video pattern recognition [4] and count the repetition times [5] and shown better performance in representing motion patterns in natural videos. Different from natural videos, cardiac imaging does not always have obvious region of interests (ROIs). Thus the motion annotations are not easily available without extra monitors or markers. Given the phase boundaries of one repetitive motion, we proposed a deep convolutional network architecture. It automatically encodes the spatial features and learns temporal repetitive patterns, to embed high dimensional video data to lower dimensional 1D curve. The softened ECG signals were used as the pseudo targets to learn the repetitive motion manifolds embedding transformation function. Hereby, simple frequency filters enable to detect and separate cardiac and respiratory motion manifolds. In this study, we aim to recover repetitive cardiac and respiratory motion using deep learning model, without full annotations and hypothesis of the explicit motion model.

¹Disclaimer: This feature is based on research, and is not commercially available. Due to regulatory reasons its future availability cannot be guaranteed

2 Methods

2.1 Input and Output Definition

Mapping ECG to cardiac phase can be noisy. As a result, we only used phase boundaries (peaks) to train the network. We applied QRS wave detection algorithm [6] to detect the peaks of the ECG signals for each cardiac video. The peak indices in X-ray fluoroscopic video p_X were $p_X = \lfloor p_E \times f_X / f_E \rfloor$, given ECG sampling rate f_E and X-ray fluoroscopic frame rate f_X and the peak index in ECG signal p_E . We labeled the middle point of the two peaks was labeled as -1 and the peaks as 1. Assuming the underlying motion phase was smooth, we assigned the labels of the intermediate frames by linear interpolation. Then, we applied a sine transformation $\hat{x} = \sin(x)$ to make smoother targets [7] as the outputs. Notably, the outputs signal were not periodic, which meant the intervals between two peaks varied. Inputs were cropped video sub-sequences of equal length.

2.2 Repetitive Motion Estimation Network (RMEN)

The network architecture was shown in Fig 1. It has 5 parts (denoted in different colors). The first weight sharing part was designed for encoding the spatial feature. Max pooling layers followed after the 1st, 3rd, and 5th Conv2D blocks. In the second part, the encoded frame features sequence then were passed to a 2-layer stacked ConvLSTM [8]. In the third part, a Conv3D layer convoluted across the channels for feature fusion. In the fourth part, the feature map encoded after Conv3D at each time point layer was flattened and passed to 3 fully connected layers, to regress the predicted phase. Mean squared error was used as the loss function. Dropout layers were added with ratio 0.5 after the first and the second dense layer to avoid overfitting. For each these frames, we had a prediction distribution $\{y^1, y^2, \dots, y^Q\}$, where y^q meant the prediction value when the frame is q^{th} visited. We always kept the median values of the prediction distributions to generate the predicted phase curve. In the last part, we detected cardiac peaks from the filtered signals.

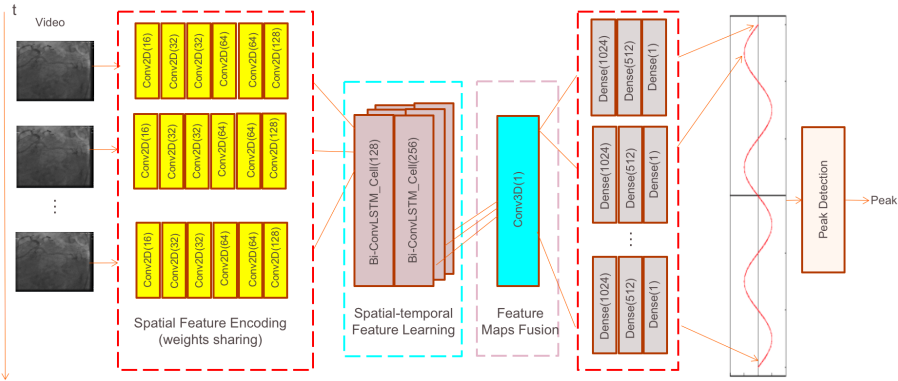


Figure 1: The architecture of Repetitive Repetitive Motion Estimation Network (RMEN)

2.3 Cardiac and Respiratory Signal Decomposition Algorithm

Although, there is no ground truth label for respiratory signal learning, we believe RMEN can learn the repetitive motion manifolds embedding function. Given the prior knowledge - the cardiac rate is around $0.5 - 2$ Hz and the respiration rate is around around $0.2 - 0.33$ Hz, we designed frequency filter to separate cardiac and respiratory signals from the predicted curve in 2.2. Defining $H(\omega, \omega_0) = 0$ when $\omega < \omega_0$, else $H(\omega, \omega_0) = 1$, the zero phase shift band-pass filter : $G(\omega) = 1 - H(\omega, \omega_h) + H(\omega, \omega_l)$, was designed to filter out cardiac signal, where ω_l is low cutoff frequency ($\omega_l = 0.5$ Hz in our application), ω_h is high cutoff frequency ($\omega_h = 2$ Hz in our application). For filtering the breathing signal, a the zero phase shift low pass filter: $G(\omega) = 1 - H(\omega, \omega_b)$ was designed, where ω_b is respiration cutoff frequency ($\omega_b = 0.33$ Hz in our application). Naive peak detection algorithm [9] was applied on cardiac phase curve for peak detection.

Table 1: Peak Detection Results (window size = 20)

Train	Test	Model	Offset/frame	True Negative	False Positive	Total
<i>A</i>	<i>B</i>	RMEN	0.88	3	27	1703
<i>A</i>	<i>B</i>	PCA+LSTM	2.16	9	72	1703
<i>A</i>	<i>B</i>	PCA+SVR	2.67	5	80	1703
N/A	<i>B</i>	DensityFlow	3.7	2	96	1703

3 Experiments and Results

3.1 Cardiac/Respiratory Signal Recovery

We used two datasets, which covered different types of cardiac procedures to evaluate our model. The model was trained on the dataset *A*, which contained 629 15fps fluoroscopic videos. We split 500 videos as the training set, 169 videos as the validation set for choosing the early stopping epoch. We tested the model on the dataset *B*, which contained 329 15fps fluoroscopic videos. Some example results are shown in 2. RMEN also could handle the irregular cardiac and respiratory motion cases, such as video shifting, skipping cardiac cycle or breathing holding, etc.

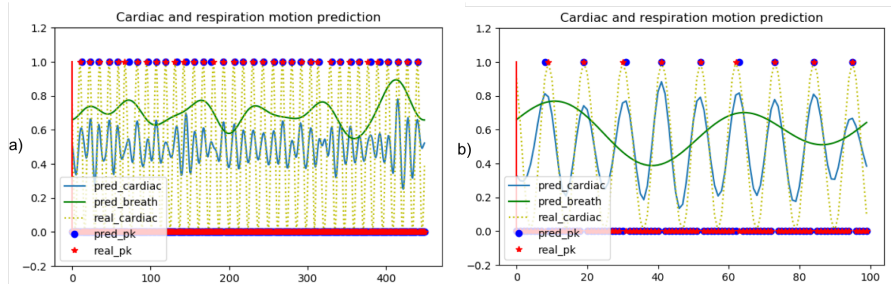


Figure 2: Cardiac (blue line) and respiratory (green line) signals decomposed from predictive curve.

3.2 Cardiac Peak Detection Model Comparison

We compared RMEN with naive LSTM and Support Vector Machine Regression (SVR), which took the 1D vector as input. The input to the naive LSTM models were flattened to a 1D vector. We used principal component analysis (PCA) based dimensional reduction. The dimension-reduced vector accounted for more than 95% of the variance of the original vector with 50 components. The best parameters for each alternative model was selected by validation. In addition, we compared with unsupervised learning methods, using the density change of the frame as signal. The model comparison results are shown in Table 1.

3.3 Visualizing Repetitive Patterns

In order to understand what RMEN learned, we examined the feature maps of the Conv3D layers (Figure 3). The results indicated repetitive patterns over time, which highlighted the change of coronaries (related to cardiac motion) and diaphragm (related to respiratory motion).

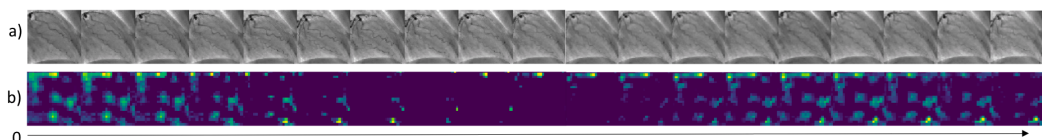


Figure 3: a): video sequence; and b)corresponding repetitive feature map of Conv3D layer

4 Conclusion

Our proposed deep learning pipeline significantly outperforms the alternative models in motion phase boundary detection. We found the repetitive patterns of cardiac and respiratory motion from the feature maps. The proposed RMEN embedded the repetitive motion manifolds to 1D signal, hence even the motions without annotation could be simply separated by frequency filtering. The proposed methods can be applied to a variety of intervention applications, such as dynamic coronary roadmapping and cardiac pacemaker tracking. It offers a solution to uncover repetitive motions, as long as the motion is smooth and partial annotations of motion boundaries are available.

References

- [1] J. R. McClelland, D. J. Hawkes, T. Schaeffter, and A. P. King, "Respiratory motion models: A review," *Medical image analysis*, vol. 17, no. 1, pp. 19–42, 2013.
- [2] D. A. Low, T. Zhao, B. White, D. Yang, S. Mutic, C. E. Noel, J. D. Bradley, P. J. Parikh, and W. Lu, "Application of the continuity equation to a breathing motion model," *Medical physics*, vol. 37, no. 3, pp. 1360–1364, 2010.
- [3] G. Shechter, J. R. Resar, and E. R. McVeigh, "Displacement and velocity of the coronary arteries: cardiac and respiratory motion," *IEEE Transactions on Medical Imaging*, vol. 25, no. 3, p. 369, 2006.
- [4] A. Karpathy, G. Toderici, S. Shetty, T. Leung, R. Sukthankar, and L. Fei-Fei, "Large-scale video classification with convolutional neural networks," in *Proceedings of the IEEE conference on Computer Vision and Pattern Recognition*, pp. 1725–1732, 2014.
- [5] O. Levy and L. Wolf, "Live repetition counting," in *Proceedings of the IEEE International Conference on Computer Vision*, pp. 3020–3028, 2015.
- [6] C. Carreiras, A. P. Alves, A. Lourenço, F. Canento, H. Silva, A. Fred, *et al.*, "BioSPPy: Biosignal processing in Python," 2015–. [Online; accessed <today>].
- [7] G. Hinton, O. Vinyals, and J. Dean, "Distilling the knowledge in a neural network," *arXiv preprint arXiv:1503.02531*, 2015.
- [8] S. Xingjian, Z. Chen, H. Wang, D.-Y. Yeung, W.-K. Wong, and W.-c. Woo, "Convolutional lstm network: A machine learning approach for precipitation nowcasting," in *Advances in neural information processing systems*, pp. 802–810, 2015.
- [9] E. Jones, T. Oliphant, P. Peterson, *et al.*, "SciPy: Open source scientific tools for Python," 2001–.