

Graphene-based Analytical Lab-on-Chip Devices for Detection of Viruses: A Review

Joydip Sengupta¹, Arpita Adhikari² and Chaudhery Mustansar Hussain^{3}*

¹Department of Electronic Science, Jogesh Chandra Chaudhuri College, Kolkata - 700033, India

²Department of Electronics and Communication Engineering, Techno Main Salt Lake, Kolkata-700091, India

³Department of Chemistry and Environmental Science, New Jersey Institute of Technology, USA

*Corresponding author Email: chaudhery.m.hussain@njit.edu

Abstract:

Lab on a chip (LOC) device intakes fluid and makes it flow through the microchannels, to achieve rapid, highly sensitive and low-cost analysis with significant yield. Graphene has vast potential to be used in LOC devices owing to its remarkable and unique properties. A trustworthy, swift, inexpensive and facile detection scheme is of urgency due to the current situation of COVID-19 to break the chain of transmission and lab-on-chip based biosensor has materialized itself as a realistic solution for this purpose. The addition of graphene has augmented the sensing capability of the LOC devices to a superior level. Recently, graphene-based lab-on-chip type biosensor is effectively used for faithful detection of SARS-CoV-2 and this draws the attention of the researchers to review the recent progress in graphene-based LOC platforms for detection of viruses and the same has been reviewed here.

Keywords: Graphene, Lab-on-chip, Biosensor, COVID-19, Virus detection

1. Lab-on-a-chip: Materials and Fabrication

“Miniaturization” has created a revolution in electronic devices by downsizing them from microelectronics to nanoelectronics. Primarily, Moser et al.¹ coined the term “Lab on Chip”

to describe the miniaturized thin-film biosensors build-up by them. Afterwards, the term LOC symbolizes a microfluidics technology-based miniaturized device that can be scaled down and also able to assimilate various laboratory operations onto a structure that can be fitted on a chip.

Various types of inorganic, organic and composite materials are employed to fabricate basic structure LOC devices. Among semiconductors, silicon is employed as the base material for LOC² owing to its good chemical stability, structural tunability and medical compatibility. To cut off the large production cost of Si, glass is also employed to build LOC devices having the additional advantage of optical transparency over Si. Among the other materials, low-temperature cofired ceramic (LTCC)³ is also used. Various types of organic materials are often employed to fabricate LOC devices such as polymer, paper and hydrogel. Among polymers, two kinds of polymers namely, elastomers and thermoplastic are used. As the performance of the LOC devices largely depends on the fabricated structure, thus, numerous aspects of LOC, along with the required fabrication material was reviewed⁴ and the results indicated that the inclusion of nanomaterials will enhance the performance of the LOC⁵ irrespective of the material used for structural development. Consequently, various nanomaterials were used in LOC⁶ for performance improvement, however, graphene becomes peerless in terms of its inclusion in LOC⁷ owing to its novel structure and exotic physio-chemical characteristics.

Regarding the fabrication techniques, both top-down and bottom-up methods are employed. Alongside top-down or bottom-up, many sub-processes such as etching, lithography, thermoforming, molding, hot embossing, polymer ablation, polymer casting, bonding are also involved in the final fabrication of the LOC device (Fig 1).

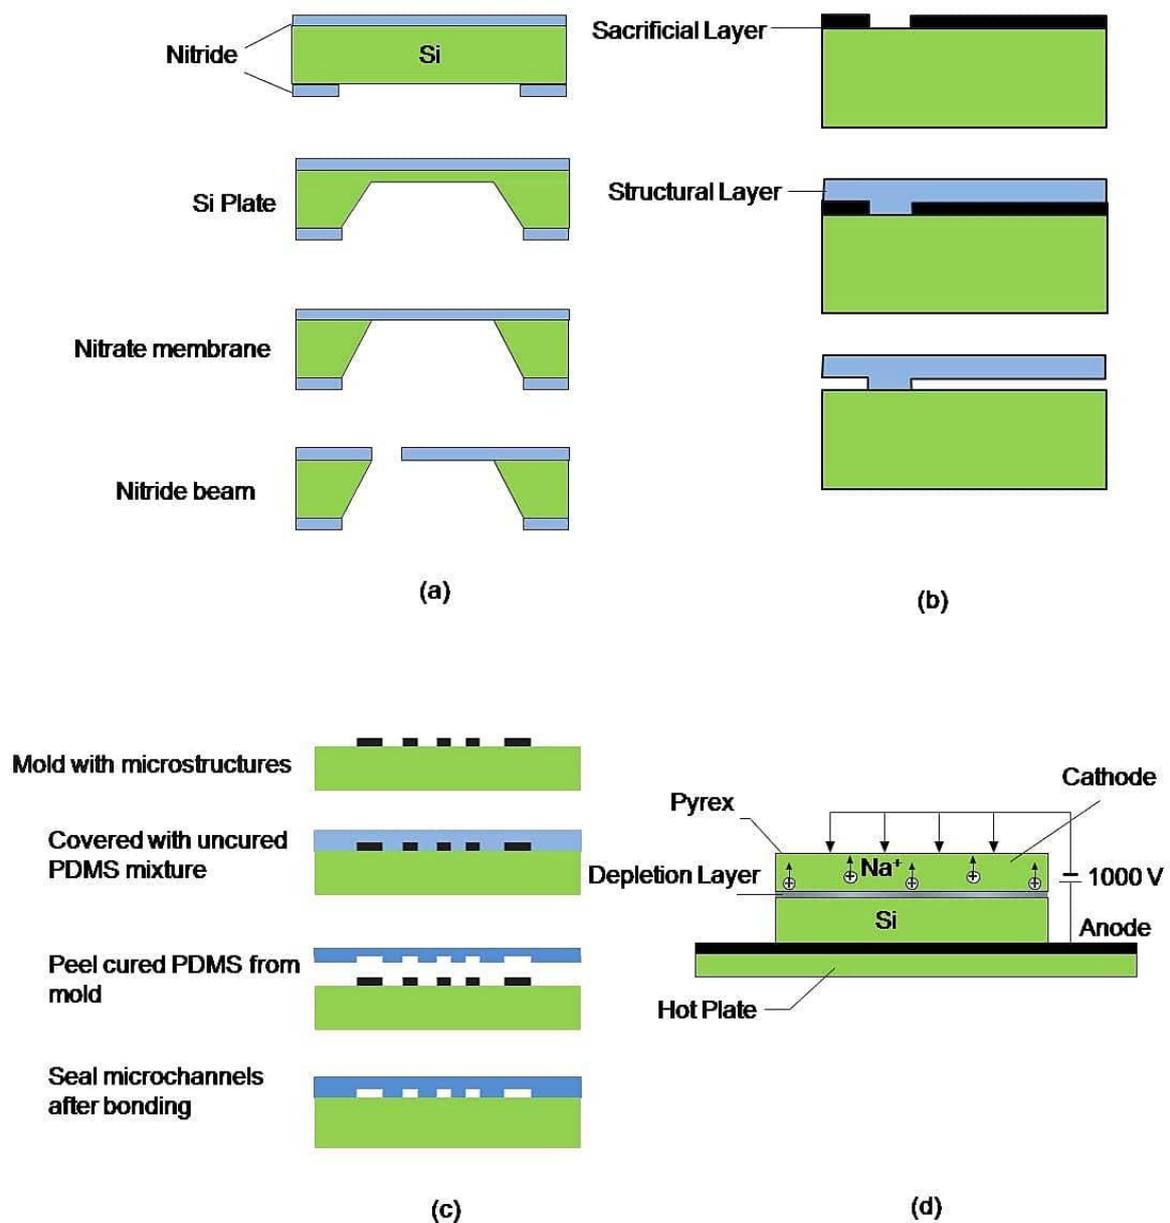


Fig 1. Different routes LOC fabrication: a) Bulk Micromachining, b) Surface Micromachining, c) SoftLithography, d) Bonding⁸.

2. Graphene: Synthesis and application as a lab-on-chip material

The production procedure and performance of the LOC device are governed by microfluidic technology and the raw material required for the fabrication of such devices should possess some distinct characteristics⁹. In addition, it was also suggested that nanomaterials such as graphene will be the preferred candidate for LOC device fabrication¹⁰. The honeycomb

structure of ultra-lightweight graphene has novel chemical and physical properties¹¹ likewise extreme optical transparency, outstanding mechanical properties, exceptionally high thermal conductivity, superior electron mobility etc (Fig 2).

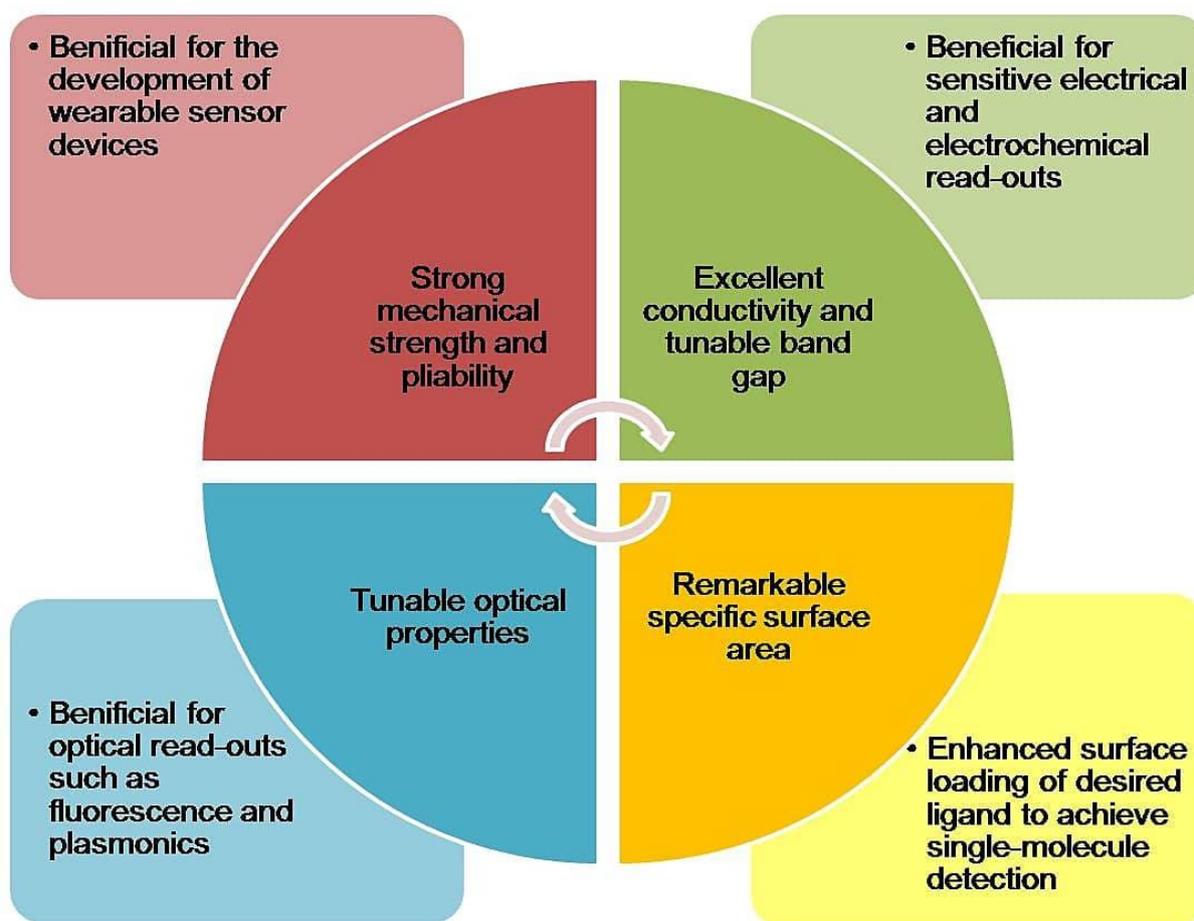


Fig 2. Novel physical and chemical properties of graphene-based materials facilitate their use in LOC platforms¹².

The mechanical strength of graphene is very high and it also has the property of pliability. The value of its Young's modulus is 1.0 terapascals with an intrinsic strength of 130 gigapascals, and breaking strength of 42 N/m¹³. The outstanding mechanical strength makes graphene an important material for the fabrication of wearable LOC devices¹⁴. In addition, graphene possesses excellent electrical conductivity along with a tunable bandgap¹⁵. Till

today, graphene is being considered as the most conductive material¹⁶ having a room-temperature electron mobility of $2 \times 10^5 \text{ cm}^2 \text{ V}^{-1} \text{ s}^{-1}$ with a conductivity of $2.12 \times 10^5 \text{ S/m}$ ¹⁷. These proved beneficial for sensitive electrical and electrochemical read-outs of LOC devices. Graphene also depicts a remarkable specific surface area¹⁸ of $2630 \text{ m}^2/\text{g}$ which helps surface loading of the desired ligand to achieve single-molecule detection in LOC devices. Moreover, graphene exhibits tunable optical properties¹⁹ which are very much advantageous for optical readouts in the case of fluorescence and plasmonic-based LOCs. Graphene also fits well within basic microfluidic fabrication techniques and thus extensively integrated with LOC devices. Thus, graphene along with its derivatives (graphene oxide (GO), reduced graphene oxide (rGO), graphene quantum dots (GQD)) are immensely employed for the fabrication of LOC²⁰. Alike most nanomaterials, graphene can be synthesised using both top-down or bottom-up technologies. In the top-down category micromechanical exfoliation, electrochemical exfoliation, thermal exfoliation of graphite intercalation compounds, reduction of GO, arc discharge and unzipping of carbon nanotubes are the techniques that are used for the fabrication of graphene. While sonication, pyrolysis, chemical vapour deposition are considered as the bottom-up methods for graphene synthesis (Fig 3).

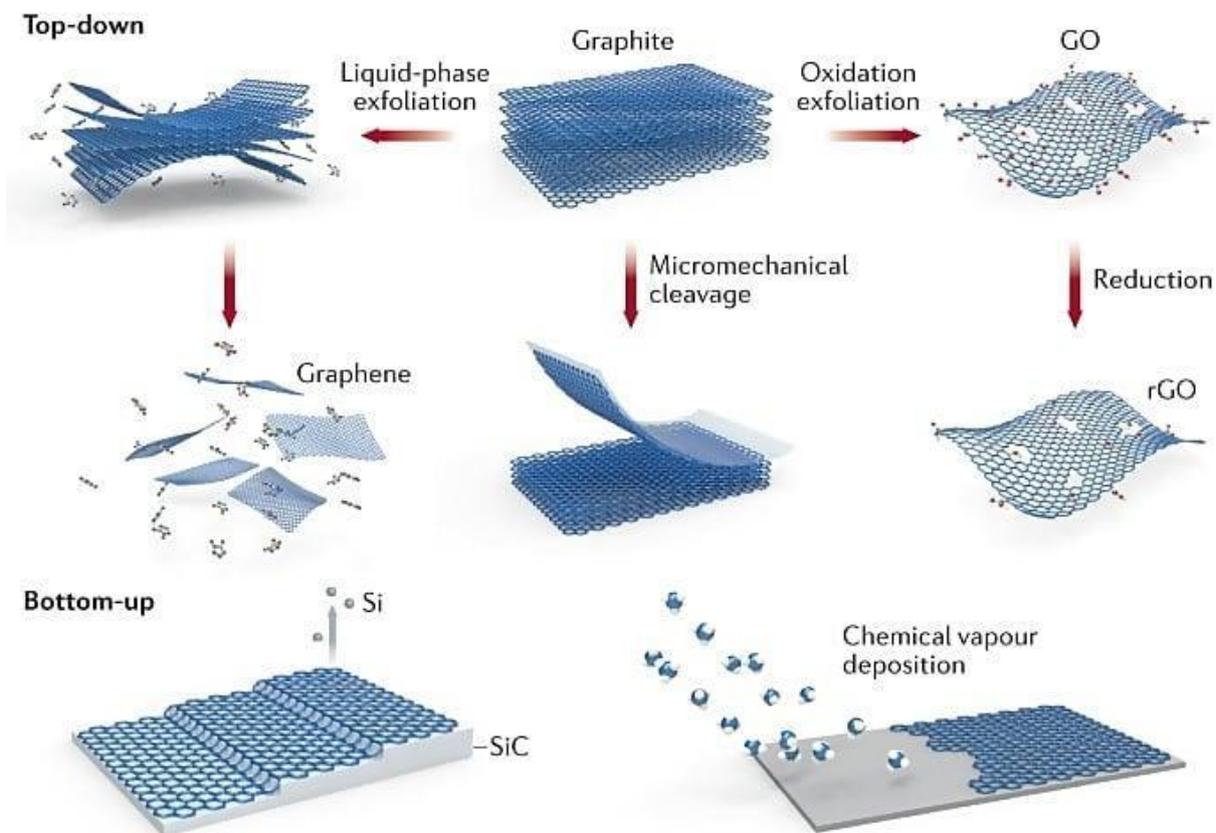


Fig 3. Various synthesis methods of graphene²¹.

In recent times scientists have devised an advanced graphene synthesis process to curb the cost of production^{22,23} up to 95.5%²⁴ and to achieve it they used ultra-low-cost carbon sources²⁵. The low production cost of graphene makes it more preferential for the fabrication of inexpensive LOC platforms with superior performance (Fig 4).

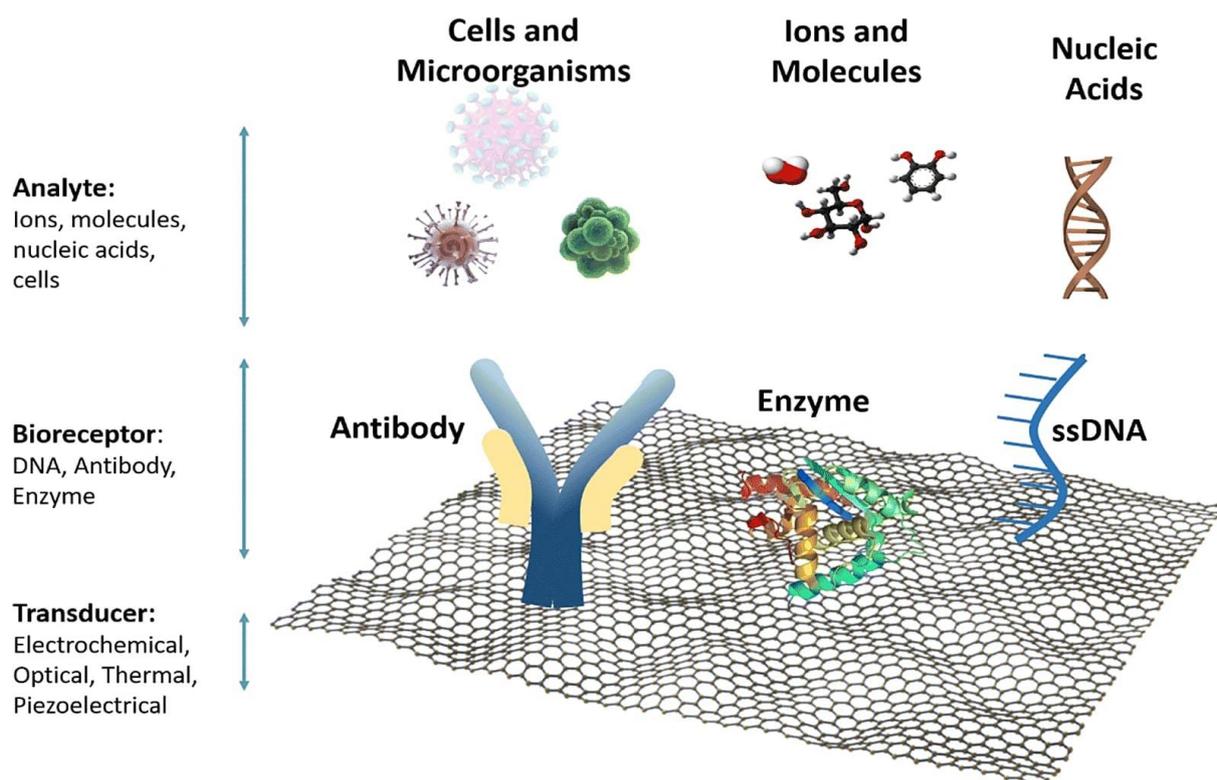


Fig 4. Various schemes of graphene-based LOC platforms for sensing²⁶.

The graphene grown by the above-mentioned methods is utilized in various LOC platforms to perform chemical, biological and point of care analysis. However, only the graphene-based analytical LOC devices used for the detection of viruses are reviewed in this paper.

3. Graphene-based lab-on-chip platforms for detection of viruses

Recently, some reviews were published where the use of LOC devices for the detection of only respiratory viruses²⁷ and the feasibility of using LOC devices for the detection of SARS-CoV-2²⁸ have been discussed. The graphene-based analytical LOC devices were reported to be employed for the detection of a wide range of viruses' starting from years old Influenza virus to current SARS-CoV-2. Thus, the widest possible range of viruses that are detectable by graphene-based analytical LOC devices is encompassed in this review.

3.1 Influenza virus

Nanoparticles of noble elements are widely used along with graphene for the detection of viruses. Huang et al.²⁹ prepared a sandwich-type immunosensor for the detection of avian influenza virus H7 (AIV H7) employing graphene coated with silver nanoparticles with a lower limit of detection (LOD) of 1.6 pg/mL. Anik et al.³⁰ employed graphene-gold hybrid nanocomposite to build an electrochemical biosensor for the detection of influenza based on a modified Au-screen printed electrode. The electrochemical route was also used by Veerapandian et al.³¹ to fabricate a dual-sensor LOC platform consists of methylene blue-electroadsorbed GO nanostructures modified with antibodies for the detection of influenza A virus at the picomolar level and the response time was extremely small. Chan et al.³² proposed a unique flow-through microfluidic approach for the detection of influenza virus gene employing rGO based transistor exhibiting LOD of 5 pM with high stability and sensitivity. The microfluidic approach was also adopted by Singh et al.³³ to fabricate rGO based electrochemical immunosensor for the detection of H1N1 with LOD of 0.5 PFU mL⁻¹ (Fig 5). The cost of the sensor has always been a major issue to make it market-ready. Working in that direction, Joshi et al.³⁴ devised a green approach for the fabrication of inexpensive, scalable thermally decomposed rGO flakes for the detection of influenza virus H1N1 with high stability and reproducibility. The functionalization of graphene has provided a new avenue towards biomolecule detection and Roberts et al.³⁵ used it to develop functionalized graphene-based field-effect transistor (GFET) for the detection of avian influenza virus with LOD 10fM. GFET biosensor structure modified with the sugar chain was employed by Matsumoto et al.³⁶ for the detection of both the human and avian influenza virus. The same group³⁷ used a glycan functionalized GFET biosensor for the detection of both the human and avian influenza virus with a LOD of 130 pM and 600 nM, respectively. GFET was also used by this group³⁸ for the detection of the influenza virus present in the

patient's saliva. A Micro-electromechanical system (MEMS) has a wide range of application including biosensor. Chen et al.³⁹ used this technique to develop a portable GFET biosensor for the detection of the H1N1 virus with a LOD of 1 ng/ml. The fluorometric approach was used by Jeong et al.⁴⁰ to fabricate a detection system for influenza virus detection. Multifunctional plasmonic/magnetic graphene was prepared by Lee et al.⁴¹ displayed unique plasmonic and magnetic effects that can be used for the detection of the Influenza virus. The detection technique was highly selective with a lower detection limit of 6.07 pg/ml in human serum. Kinnamon et al.⁴² developed a novel screen printed GO-based textile biosensor with high reproducibility and stability. The fabricated biosensor depicted a LOD of 10 ng/mL.

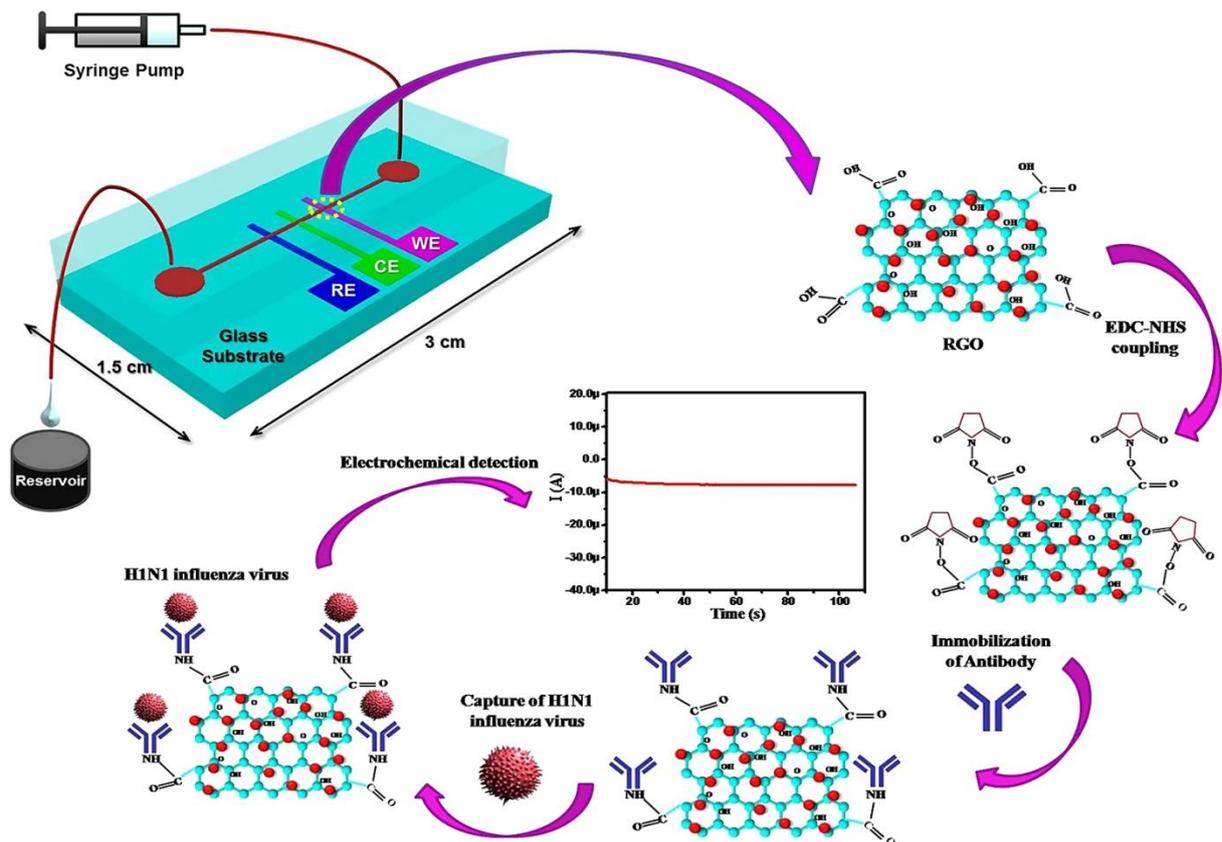


Fig 5. Schematic illustration of the microfluidics-integrated electrochemical immunosensing chip coated with RGO, followed by antibody immobilization using EDC/NHS coupling for the detection of influenza virus H1N1⁴³.

3.2 Ebola Virus

Fu et al.⁴⁴ used GO to design a supramolecular fluorogenic peptide sensor array for the detection of the Ebola virus. The methods depicted high selectivity in detecting the Ebola virus even in the presence of the Marburg virus and vesicular stomatitis virus. Virus detection using fluorescence quenching property of GO along with rolling circle amplification was employed by Wen et al.⁴⁵ to detect the Ebola virus with LOD 1.4 pM both in aqueous solution and 1% serum solution. GFET type biosensors are extensively employed for the detection of the Ebola virus. Maity et al.⁴⁶ developed rGO based GFET and used the electronic-resonance frequency, namely inflection frequency to detect the Ebola virus. The sensitivity of the used methodology is several orders of magnitude higher than the sensitivity from other electronic parameters. The Ebola virus was detected by Jin et al.⁴⁷ by monitoring the response of the rGO based GFET as a function of the Dirac voltage with LOD of 2.4 pg/mL. Chen et al.⁴⁸ developed the rGO based GFET structure and tested the sensor's performance with Ebola virus antigens suspended in $0.01 \times$ PBS/human serum/plasma and the result showed that the device could successfully detect the Ebola virus with the LOD of 1 ng/ml.

3.3 Dengue Virus

Jin et al.⁴⁹ designed a surface-based impedimetric biosensor using self-assembled functionalized GO wrapped SiO₂ particles for label-free detection of dengue virus with LOD 1fM. Opto-electrochemically active ruthenium bipyridine complex was attached to the surface of GO by Kanagavalli et al.⁵⁰ for the detection of the dengue virus. The immunosensor showed a linear response both under the chronoamperometric and fluorescence quenching-based immunoassays with a LOD of 0.38 and 0.48 ng/mL,

respectively. For the detection of the dengue virus, Omar et al.⁵¹ developed an optical biosensor using surface plasmon resonance of CdS quantum dots composited with amine-functionalized GO thin film, which exhibited a LOD of 1 pM with a sensitivity of 5.49° nM⁻¹. They also reported similar biosensing techniques^{52, 53} using rGO- polyamidoamine nanocomposite which showed a better performance with LOD of 0.08 pM for the detection of dengue virus. The fluorometric approach was adopted by Lee et al.⁵⁴ and integrated with a loop-mediated isothermal amplification assay to increase the overall sensitivity of the GO-based biosensor for the detection of dengue with LOD 2.1 nM. Kamil et al.⁵⁵ employed a GO integrated biofunctionalized tapered optical fibre based sensor to detect the dengue virus with a LOD of 1 pM along with the sensitivity of 12.77 nm/nM. Electrochemical impedance spectroscopy was employed by Navakul et al.⁵⁶ using GO reinforced polymer to detect the dengue virus with a 0.12 pfu/mL detection limit.

3.4 SARS-CoV-2 Virus

Graphene was functionalized with SARS-CoV-2 spike antibody by Seo et al.⁵⁷ to fabricate a biosensor for the detection of SARS-CoV-2. To immobilize the SARS-CoV-2 spike antibody on GFET they used 1-pyrenebutanoic acid succinimidyl ester as a probe linker. The detection of SARS-CoV-2 using the fabricated device is possible both in the transport medium and clinical sample with a LOD of 1 fg/ml. GFET structure fabricated by Zhang et al.⁵⁸ can detect SARS-CoV-2 within 2 mins with a LOD of 0.2 pM. Alafef et al.⁵⁹ devised a way for quick, quantitative, inexpensive and ultrasensitive detection of SARS-CoV-2 employing a graphene-based electrochemical biosensor chip containing Au nanoparticles. The performance of the biosensor chip was checked using both SARS-CoV-2 infected Vero cell samples and clinical samples and the chip exhibited a sensitivity of 231 (copies μL^{-1})⁻¹ and LOD of 6.9 copies/ μL

(Fig 6). Simone et al.⁶⁰ theoretically studied the possibility of using a graphene-based optical sensor for the detection of SARS-CoV-2 employing Raman scattering. An ultrasensitive supersandwich-type electrochemical sensor was developed by Zhao et al.⁶¹ employing calixarene functionalized GO to detect RNA of SARS-CoV-2. The fabricated device showed a LOD of 200 copies/mL with the clinical specimen moreover, it needs a very small amount of sample (only two copies of SARS-CoV-2) for faithful detection. Hashemi et al.⁶² constructed a nanosensor based on the GO-Au nanoparticle to detect the trace of SARS-CoV-2 in any aquatic biological media via the interaction with the active functional groups of their glycoproteins. The device can detect SARS-CoV-2 within 1 min and having the LOD of $1.68 \times 10^{-22} \mu\text{g mL}^{-1}$. Rodríguez et al.⁶³ devised a unique graphene-based multiplexed immunosensor telemedicine platform employing laser-engraved graphene. The device can perform highly selective, ultrasensitive, and rapid electrochemical detection of SARS-CoV-2 in blood and saliva samples. A paper-based electrochemical immunosensor for the detection of SARS-CoV-2 was fabricated by Yakoh et al.⁶⁴ employing GO. The device can detect SARS-CoV-2 in real clinical sera from COVID patients with LOD of 1 ng/mL and also capable of SARS-CoV-2 antigen detection. Samavati et al.⁶⁵ used Au/fiber Bragg grating probe decorated with GO to detect the SARS-CoV-2 virus from patients' saliva and the disease level is identified by the deviation of wavelength and amplitude from healthy saliva. Superfast detection of COVID-19 antibody was made possible by Ali et al.⁶⁶ using aerosol jet nanoprinted rGO nanoflakes-coated 3D electrodes integrated with a microfluidic device. The impedance spectroscopy was used to detect the change in impedance upon the presence of SARS-CoV-2 with LOD of $2.8 \times 10^{-15} \text{ M}$ which can be monitored via a smartphone-based user interface.

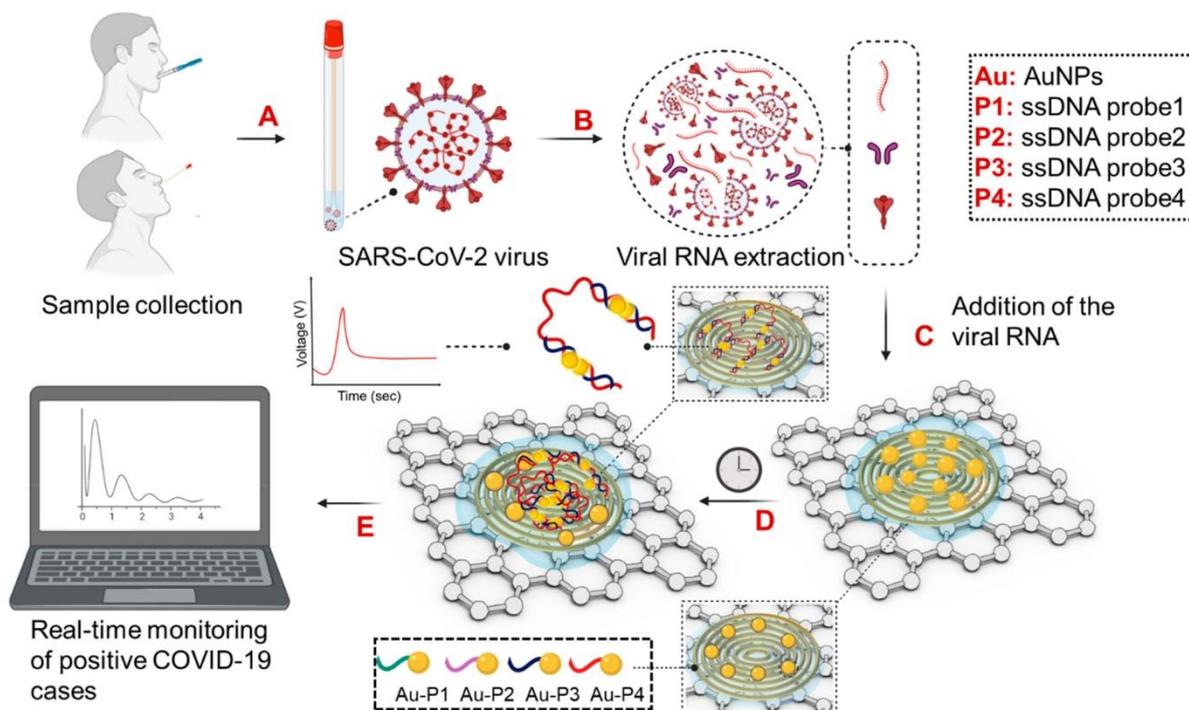


Fig 6. Scheme 1. Schematic representation of the operation principle of the COVID-19 electrochemical sensing platform wherein step A: the infected samples will be collected from the nasal swab or saliva of the patients under observation; step B: the viral SARS-CoV-2 RNA will be extracted; step C: the viral RNA will be added on top of the graphene-ssDNA-AuNP platform; step D: incubation of 5 min; and step E: the digital electrochemical output will be recorded⁶⁷.

3.5 Rotavirus

Liu et al.⁶⁸ combined the Hummers method, photolithography and reduction process to fabricate micropatterned rGO FET to detect rotavirus with LOD of 10^2 pfu. The same group also developed an electrochemical biosensor⁶⁹ using GO thin film modified with pyrene derivatives for the detection of rotavirus. Chemi-resistive rGO FET biosensor was developed by Pant et al.⁷⁰ and employed pyrene-NHS (Linker) complex to attach the antibodies on the channel of the FET structure for the detection of rotavirus. Fan et al.⁷¹ devised a process for effective detection and removal of rotavirus from infected water using a bioconjugated magnetic nanoparticle-attached hybrid GO-based 3D plasmonic-magnetic solid architecture. Jung et al.⁷² developed a GO-based immunobiosensor system to detect norovirus employing

fluorescence quenching effect between GO and Au nanoparticle. The maximized GO quenching efficiency was obtained up to 85% at 10^5 pfu/mL.

3.6 Hepatitis B Virus

Gold nanoparticle combined with graphene plays a significant role in the detection of hepatitis B virus. Huang et al.⁷³ modified graphene electrode with gold nanoparticles and a Nafion-L-cysteine composite film to construct a stable and sensitive electrochemical immunosensor for the detection of hepatitis B with LOD of 0.1 ng mL^{-1} . GO-gold nanorod composite was used by Liu et al.⁷⁴ for tracing the presence of hepatitis B virus in serum employing surface-enhanced Raman spectroscopy. The fabricated device is specific and highly selective with a LOD of $0.05 \text{ pg}\cdot\text{mL}^{-1}$. Muain et al.⁷⁵ used rGO decorated with gold nanoparticle for impedimetric detection of hepatitis B virus with LOD of 3.80 ng mL^{-1} . Graphene resistor, modified with self-assembled graphene-gold nanoparticles was used to sense hepatitis B virus with LOD of 50 pg mL^{-1} by Walters et al.⁷⁶. An electrochemical aptasensor was constructed by Mohsin et al.⁷⁷ by modifying the surface of a glassy carbon electrode with gold nanoparticles functionalized rGO. The fabricated device showed an extremely superior LOD of 0.0014 fg/mL . Zhao et al.^{78, 79} constructed a label-free immunosensor using multilayer film of GO/ferrocene-chitosan nanocomposite and gold nanoparticles for the detection of hepatitis B virus with LOD of 0.01 ng/mL . GQDs are also used for the detection of hepatitis B virus likewise Xiang et al.⁸⁰ used GQD based electrochemical biosensing platform that depicts high sensitivity with a LOD of 1 nM . Tan et al.⁸¹ prepared new nanoenzymes using PdCu tripod functionalized porous graphene for the fabrication of hepatitis B biosensor with high selectivity, good stability and reproducibility. The LOD of the constructed biosensor was $20 \text{ fg}\cdot\text{mL}^{-1}$. GFET structure also finds its way in

the successful detection of the hepatitis B virus. Ray et al.⁸² used a probabilistic neural network (PNN) for the detection of hepatitis B virus using GFET biosensor. The use of the PNN method showed better performance than its peers and thus lowering the detection limit of the Hepatitis B virus down to 0.1 fM. The nanoporous SiO₂ template was employed by Basu et al.⁸³ to develop an rGO based GFET for sensing the hepatitis B virus to achieve a LOD of 50aM.

3.7 Hepatitis C Virus

Kim et al.⁸⁴ devised a novel, cost-effective and stable delivery system based on nano GO for simultaneous detection and inhibition of Hepatitis C. The detection was enabled by the DNAzyme-nano GO complex system while DNAzyme mediated catalytic cleavage performed the inhibition of the virus. The silver nanoparticle was employed by Valipour et al.⁸⁵ along with GQD to form a nanocomposite platform with a large surface area for the detection of hepatitis C with a LOD of 3 fg mL⁻¹. For the quantitative detection of Hepatitis C core antigen, they introduced Riboflavin as a redox probe. Fan et al.⁸⁶ employed a fluorescence-based method for the detection of Hepatitis C using rGO nanosheets along with a hybridization chain reaction amplification technique. They studied biological samples under complicated environments and their method exhibited a LOD of 10 fM. Li et al.⁸⁷ developed a novel nanocomposite of DNA assisted magnetic rGO-Cu for highly sensitive detection of the Hepatitis C virus. The sensing with a LOD of 405 pM was accomplished using the electrochemical signal originated by Cu²⁺ catalyzed oxidation of O-phenylenediamine. A unique nanocomposite consisting of cucurbit[7]uril and graphene were made by Jiang et al.⁸⁸ for electrochemical sensing of Hepatitis C virus with a detection limit as low as 160.4 pmol/L.

3.8 Papilloma Virus

Huang et al.⁸⁹ employed graphene/Au nanorod/polythionine to construct an ultrasensitive, electrochemical, enzyme-free and label-free DNA biosensor for the detection of human papilloma virus DNA using electrochemical impedance spectroscopy and differential pulse voltammetry. The amplification of the electrochemical signals was achieved by the long-range self-assembly of DNA nanostructure which exhibited a LOD of 4.03×10^{-14} mol/L. Chekin et al.⁹⁰ used porous rGO/MoS₂ to modify glassy carbon electrodes for the sensitive and selective detection of the human papilloma virus employing aptamers as recognition elements. The fabricated electrochemical sensor was able to detect the human papilloma virus with a LOD of 1.75 pM. The electrochemical sensing route was also adopted by Farzin et al.⁹¹ using CNT/amine-ionic liquid functionalized rGO nanoplateforms as a sensing interface for the detection of human papilloma virus in clinical samples with LOD of 13nM. Aptamer-functionalized rGO-FET was constructed by Aspermaier et al.⁹² to detect the human papilloma virus in saliva and the fabricated device was able to detect the virus with a LOD of 1.75 nM. Mahmoodi et al.⁹³ prepared a nanocomposite of rGO/MWCNTs and electrodeposited it on a screen-printed carbon electrode. Later on, Au nanoparticles were added and a single-strand DNA probe was immobilized on the modified screen-printed carbon electrode. The differential pulse voltammetry assay was employed for the electrochemical measurement which revealed that the biosensor can detect the virus with a LOD of 0.05 fM.

3.9 Norovirus

Graphene decorated with nanoparticles was extensively used in determining the presence of norovirus. Lee et al.⁹⁴ prepared a hybrid nanomaterial-sensing platform using Au/Fe₃O₄ decorated graphene for sensing norovirus. Owing to the high electrical conductivity and magnetic property of the hybrid structure, the sensing platform showed an exceptional sensitivity level with a LOD of 1.16 pg/ml. Ahmed et al.⁹⁵ also prepared an Au-graphene nanohybrid using chloroauric acid, sodium formate and graphene flakes for the detection of norovirus. The catalytic activity of the nanohybrid was employed for the detection of norovirus with a LOD of 92.7 pg/mL. Chand et al.⁹⁶ developed an electrochemical aptasensor based on graphene-gold nanocomposite and integrated it with the all-polydimethylsiloxane (PDMS) microfluidic chip. They used differential pulse voltammetric analysis for the sensing of norovirus in spiked blood with LOD of 100pM (Fig 7). A unique biosensing platform was developed by Achadu et al.⁹⁷ based on graphene-mediated surface-enhanced Raman scattering (SERS) using plasmonic/magnetic molybdenum trioxide nanocubes for the detection of norovirus. Molybdenum trioxide nanocubes acted as SERS nanotag while graphene acted as the signal reporter. The fabricated biosensor was used to detect norovirus in human fecal samples with a LOD of 5.2 fg/mL. 3D inkjet printed GFET was employed by Xiang et al.⁹⁸ as a flexible biosensor platform for the detection of norovirus with the limit of detection around 0.1 µg/ml. Weng et al.⁹⁹ adopted an aptamer-based fluorometric approach for the detection of norovirus employing a microfluidic device fabricated using 6-carboxyfluorescein, MWCNT and GO. The hybrid biosensing system was able to detect norovirus with LOD of 3.3 ng·mL⁻¹. GO/Fe nanocomposite was prepared by Kim et al.¹⁰⁰ for the detection of norovirus in tap water and artificial urine based on the principle of intra chemiluminescent resonance transfer with LOD of 80 ng/ml.

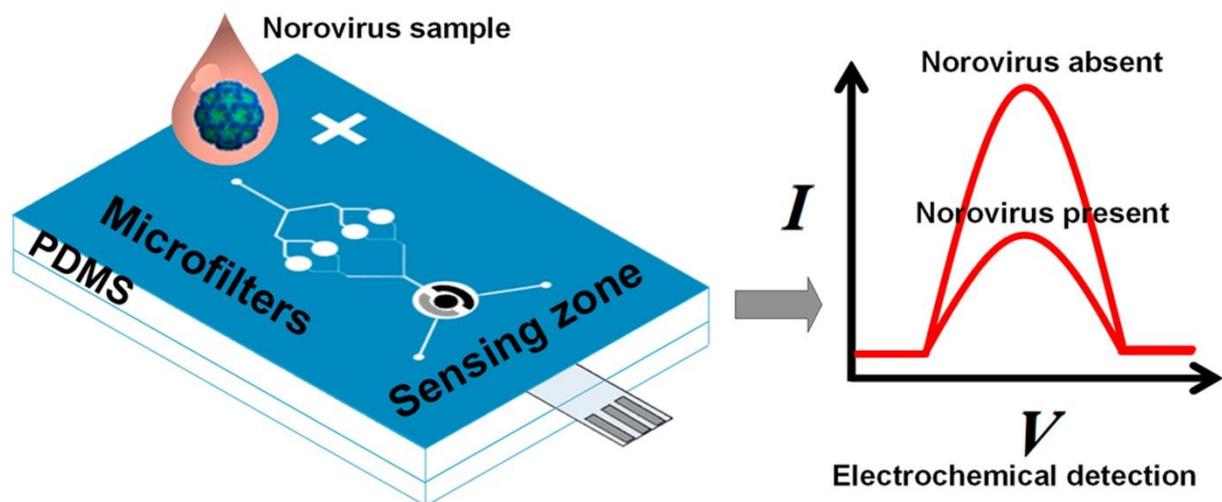


Fig 7. Microfluidic carbon electrode with Grp-AuNPs composite for Norovirus detection¹⁰¹.

3.10 Human Immunodeficiency Virus (HIV)

Gong et al.¹⁰² used rGO for the fabrication of impedimetric DNA biosensor to detect HIV with a LOD of 3.0×10^{-13} M. Later on, they modified¹⁰³ the detection approach by modifying glassy carbon electrode using rGO-nafion composite film for the detection of HIV gene with a LOD of 2.3×10^{-14} M. Here stability of graphene coating was enhanced by nafion which increases graphene dispersion. They have also used polyaniline/graphene nanocomposite and dropcasted it onto a glassy carbon electrode for HIV detection¹⁰⁴ and this time the LOD is 1.0×10^{-16} M. Detection of HIV using fluorescence polarization was achieved by Wang et al.¹⁰⁵ employing GO as a signal amplifier and the LOD of the fabricated chip was 38.6 pmol/L. Kwon et al.¹⁰⁶ used a photolithographic approach to fabricate a scalable and flexible, liquid ion-gated GFET structure and decorated it with close-packed carboxylated polypyrrole nanoparticle arrays to sense the HIV with LOD of 1 pM. Amine-functionalized graphene was employed by Islam et al.¹⁰⁷ to fabricate a GFET biosensor to detect HIV with a LOD of 10 fg/mL. Flexible polyethylene terephthalate was used as a substrate for the fabrication of coplanar-gate GFET by Kim et al.¹⁰⁸ for the detection of HIV. The GFET revealed a

remarkable LOD of 47.8 aM in detecting HIV. Vishnubhotla et al.¹⁰⁹ used CVD grown graphene along with the photolithography technique to construct a GFET aptasensor that can detect HIV with LOD of 1 ng/mL. Li et al.¹¹⁰ studied the employability of fluorescence resonance energy transfer (FRET) technique using boron and nitrogen co-doped GQD to construct a biosensing platform for the detection of HIV and the results exhibited that the device can sense HIV with LOD of 0.5 nM. FRET was also exploited to develop a GO-based sensing platform by Zhang et al.¹¹¹ for building a robust and highly sensitive biosensor for the detection of HIV in human serum with a LOD of 1.18 ng/mL. GO-polycarbonate track-etched nanosieve electrochemical biosensing platform was constructed by Nehra et al.¹¹² for the sensitive and rapid detection of HIV with LOD of 8.3 fM. Wang et al.¹¹³ constructed an electrochemical biosensing platform employing a glassy carbon electrode modified with graphene stabilized gold nanocluster, and integrated with an exonuclease III assisted target recycling amplification strategy to detect HIV with LOD of 30 aM.

3.11 Other Viruses

Photolithography along with plasma-enhanced chemical vapour deposition was employed by Afsahi et al.¹¹⁴ for the fabrication of inexpensive and portable GFET to detect Zika virus in serum which could detect the virus with LOD of 450 pM. Moco et al.¹¹⁵ opted for the electrochemical route for the fabrication of electrochemical genosensor based on graphite electrodes modified with rGO and polytyramine-conducting polymer which could detect Zika virus with LOD of 0.1 fg/mL within 20 mins. Jin et al.¹¹⁶ prepared a composite of 3-Aminopropyltriethoxysilane functionalized GO wrapped on SiO₂ particles via self-assembly to construct an impedimetric biosensor to detect the Zika virus. An electrochemical immunosensor was constructed by Li et al.¹¹⁷ using MoS₂-rGO nanocomposite decorated

with gold nanoparticles to detect the diarrhea virus. Chowdhury et al.¹¹⁸ employed GQD to construct an electrochemical LOC platform to detect hepatitis E viruses with a LOD of 0.8 fg mL⁻¹.

4. Challenges and Outlook

The advancement of medical science is not possible without modernization and accelerated clinical diagnosis. Though graphene-based LOC devices extend quick and easy detection of several viruses, yet the recent worldwide outbreak of the SARS-CoV-2 virus not only makes the scientific community realize the challenging aspects of such detection technique but also motivate them in accelerating the research to develop the existing LOC devices with advanced features like integrated-sample preparation, large yield and multiplex detection, high sensitivity or low detection error, integrability with smart devices and finally cost-effectiveness.

Any virus outbreak comes with the challenge of immediate action on impeding further transmission and chain-breaking. An integrated sample preparation capability of existing LOC devices may lead to more rapid detection of the viruses and consequently help in preventing an outbreak. Some recent research showed such incorporation of sample detection capability into LOC^{119,120}. However, consolidated graphene-based LOC with single-chip sample preparation or extraction is still lacking. Whether it is a home-based or a clinical centre-based diagnosis, futuristic automation, as well as rapid identification of viral infection, will not be possible without the advent of the LOC device. Integrated sample preparation within LOC will enable rapid detection of the infection with minimal delay and thus the patients can be offered immediate treatment to prevent a fatality.

The recent outbreak of SARS-CoV-2 exerts a thrust into clinical research highlighting several critical requirements like the multi-detection capability of LOC devices. A single viral infection often comes with multi-variant infection in human bodies leading to even loss of human life without early detection. This type of situation in medical science demands highly sensitive and multiplex detection. Consequently, multi-variant infection detection through a single chip is of utmost importance for the recent advancement of LOC devices. Moreover, in most cases, viral infections having numerous sub-types are found to spread quickly and impose a crucial challenge for LOC devices. To cater greater portion symptomatic population through a single detection chip, the graphene-based LOC devices are required to have high throughput as evidenced in the case of some of the microfluidic chips in the published literature^{121,122}. Graphene-based LOC with high throughput and multiplex detection capability can effectively decrease the cost-per-patient criterion and thereby can widen its use.

Some recent studies^{123,124} reported the efficacy of the digital quantitative method in terms of its better precision of detection in comparison to the standard quantitative method. Advanced technology like robotic process automation can be clubbed to the existing clinical LOC devices to realize “sample-in-digital-answer-out”. Nevertheless, such technology presently associated with certain limitations like cost and implementation. To cope-up with the futuristic technological advancement, the graphene-based LOCs should confront the challenge of the digital quantitative method through more rigorous multi-disciplinary research activities.

In the case of infectious diseases, the clinical diagnosis of patients with low viral load always faces a serious challenge to existing technologies. Among the available techniques, plasmonic and electrochemical probing of the clinical detection process possesses the highest sensitivity in viral load detection. Moreover, the plasmonic investigation inherits advantages

like highest throughput as well as fastest read-out among other significant assays like colorimetric, lateral flow, magnetic, and electrochemical approaches. More rigorous scientific investigation can lead to an overall improved version of LOC.

Because of the present technological evolution, the integration of existing LOC detection with smart devices is becoming an utmost requisite in modern state-of-the-art living. Recent studies had already indicated new technologies to enable the LOC to function in conjunction with smart read-out capabilities¹²⁵.

Finally, all the above-mentioned features of the LOC unit are required to be implemented in a cost-effective approach because of the large-scale spreading aspect of a virus outbreak that can even lead to another pandemic scenario without immediate attention (Fig 8).

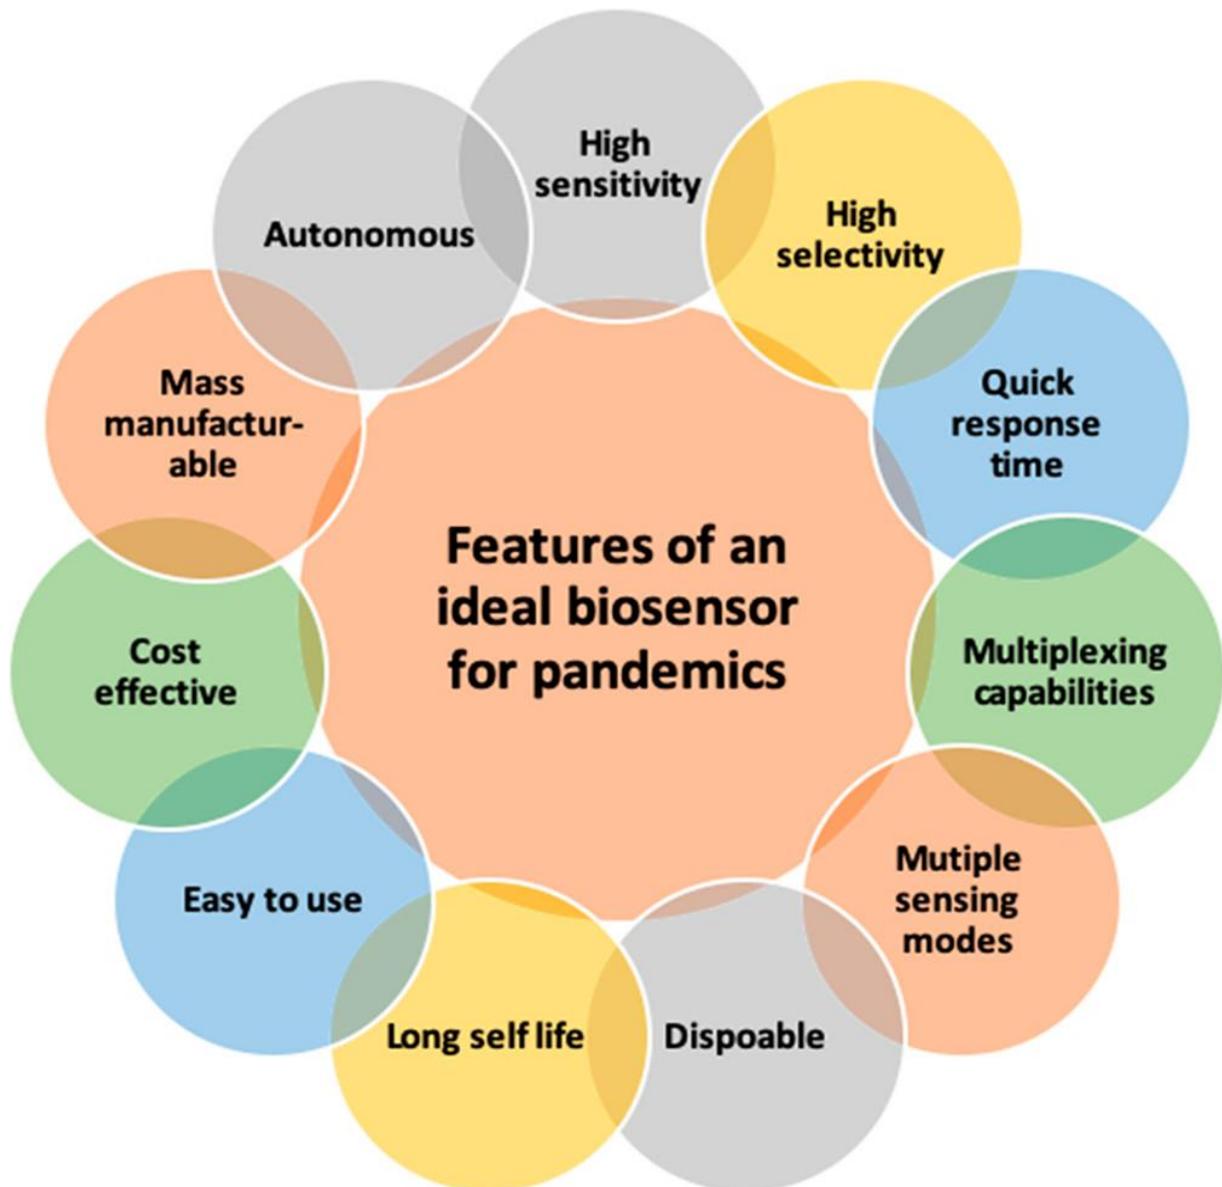


Fig 8. Features of an ideal biosensor required to be developed for effective use¹²⁶.

5. Conclusions

Graphene-based LOC devices offer the advantages of novel physiochemical properties of graphene along with exotic analytical characteristics of microfluidics namely minimal consumption of target molecules, rapid detection, user-friendliness with high sensitivity. Here, firstly the fabrication process technologies for LOC device has been discussed and thereafter advantages of using graphene in LOC devices have been explored. Later on, the application of graphene-based LOC in detecting a wide spectrum of viruses has been

reviewed which ranges from the detection of years old influenza virus to modern SARS-CoV-2. From the economic perspective, graphene depicts a huge potential as recent developments show a steep decrease in the production cost of high-quality graphene. However, still, there are some issues namely toxicity, shelf life and sustainability, which are needed to be addressed with utmost concern. Reproducibility plays a major role in any type of nanodevice and graphene-based LOC comes under it. Moreover, as graphene-based LOCs are mostly meant for point of care related application, thus the process integrity and material reproducibility need an extensive quality check. In summary, till now graphene along with its derivatives has overcome most of the hurdles, thus it can be believed that an eco-friendly, inexpensive, reproducible and sustainable graphene-based LOC platform will pave a new way for the detection of almost all kinds of viruses.

¹ I.Moser G.Jobst E.Aschauer P.Svasek M.Varahram G.UrbanV.A.ZaninG.Y.TjoutrinaA.V.Zharikova T.T.Berezov, ‘Miniaturized Thin Film Glutamate and Glutamine Biosensors’, *Biosensors and Bioelectronics* 10, no. 6–7 (1995): 527–32, [https://doi.org/10.1016/0956-5663\(95\)96928-R](https://doi.org/10.1016/0956-5663(95)96928-R).

²Yaping Zhang, ‘Optimal Design of Label-Free Silicon “Lab on a Chip” Biosensors’, *Progress in Natural Science: Materials International* 23, no. 5 (1 October 2013): 481–86, <https://doi.org/10.1016/j.pnsc.2013.09.002>.

³Petra S. Dittrich, ‘Research Highlights’, *Lab on a Chip* 7 (2007): 663–65, <https://doi.org/10.1039/b706143a>.

⁴D. Mark et al., ‘Microfluidic Lab-on-a-Chip Platforms: Requirements, Characteristics and Applications’, *Chemical Society Reviews* 39 (2010): 1153–82, <https://doi.org/10.1039/b820557b>.

⁵Martin Pumera, ‘Nanomaterials Meet Microfluidics’, *Chemical Communications* 47, no. 20 (2011): 5671–80, <https://doi.org/10.1039/c1cc11060h>.

⁶Rüstem Keçili, Sibel Büyüktiryaki, and Chaudhery Mustansar Hussain, ‘Advancement In Bioanalytical Science Through Nanotechnology Past, Present And Future’, *TrAC Trends in Analytical Chemistry* 110 (2019): 259–76, <https://doi.org/10.1016/j.trac.2018.11.012>.

⁷Mohammad Hasanzadeh et al., ‘Two Dimension (2-D) Graphene-Based Nanomaterials as Signal Amplification Elements in Electrochemical Microfluidic Immune-Devices: Recent Advances’, *Materials Science and Engineering C* 68 (2016): 482–93, <https://doi.org/10.1016/j.msec.2016.06.023>.

⁸Joydip Sengupta and Chaudhery Mustansar Hussain, ‘Graphene and Its Derivatives for Analytical Lab on Chip Platforms’, *TrAC Trends in Analytical Chemistry* 114 (1 May 2019): 326–37, <https://doi.org/10.1016/j.trac.2019.03.015>.

⁹Mark et al., ‘Microfluidic Lab-on-a-Chip Platforms: Requirements, Characteristics and Applications’.

¹⁰Pumera, ‘Nanomaterials Meet Microfluidics’.

¹¹Santosh Bahadur Singh and Chaudhery Mustansar Hussain, ‘Nano-Graphene as Groundbreaking Miracle Material: Catalytic and Commercial Perspectives’, *ChemistrySelect* 3, no. 33 (2018): 9533–44, <https://doi.org/10.1002/slct.201802211>.

¹²Joydip Sengupta and Chaudhery Mustansar Hussain, ‘Graphene-Based Field-Effect Transistor Biosensors for the Rapid Detection and Analysis of Viruses: A Perspective in View of COVID-19’, *Carbon Trends* 2 (1 January 2021): 100011, <https://doi.org/10.1016/j.cartre.2020.100011>.

¹³Changgu Lee et al., ‘Measurement of the Elastic Properties and Intrinsic Strength of Monolayer Graphene’, *Science* 321, no. 5887 (18 July 2008): 385–88, <https://doi.org/10.1126/science.1157996>.

-
- ¹⁴Altynay Kaidarova et al., 'Wearable Multifunctional Printed Graphene Sensors', *Npj Flexible Electronics* 3, no. 1 (2 August 2019): 1–10, <https://doi.org/10.1038/s41528-019-0061-5>.
- ¹⁵Yuanbo Zhang et al., 'Direct Observation of a Widely Tunable Bandgap in Bilayer Graphene', *Nature* 459, no. 7248 (June 2009): 820–23, <https://doi.org/10.1038/nature08105>.
- ¹⁶S. V. Morozov et al., 'Giant Intrinsic Carrier Mobilities in Graphene and Its Bilayer', *Physical Review Letters* 100, no. 1 (7 January 2008): 016602, <https://doi.org/10.1103/PhysRevLett.100.016602>.
- ¹⁷Leo Rizzi et al., 'Quantifying the Influence of Graphene Film Nanostructure on the Macroscopic Electrical Conductivity', *Nano Express* 1, no. 2 (September 2020): 020035, <https://doi.org/10.1088/2632-959X/abb37a>.
- ¹⁸Songdi Zhang et al., 'Measuring the Specific Surface Area of Monolayer Graphene Oxide in Water', *Materials Letters* 261 (15 February 2020): 127098, <https://doi.org/10.1016/j.matlet.2019.127098>.
- ¹⁹Feng Han et al., 'A Highly Efficient Synthetic Process of Graphene Films with Tunable Optical Properties', *Applied Surface Science* 314 (30 September 2014): 71–77, <https://doi.org/10.1016/j.apsusc.2014.05.222>.
- ²⁰Shigang Wu et al., 'Recent Advances in the Fabrication and Application of Graphene Microfluidic Sensors', *Micromachines* 11, no. 12 (December 2020): 1059, <https://doi.org/10.3390/mi11121059>.
- ²¹Xiao-Ye Wang, Akimitsu Narita, and Klaus Müllen, 'Precision Synthesis versus Bulk-Scale Fabrication of Graphenes', *Nature Reviews Chemistry* 2, no. 1 (20 December 2017): 1–10, <https://doi.org/10.1038/s41570-017-0100>.
- ²²Wazeem Nishad and Sathyan Subbiah, 'Machining Induced Transformation of Graphite Flakes to Graphite/Graphene Nanoplatelets', *Manufacturing Letters* 21 (1 August 2019): 66–69, <https://doi.org/10.1016/j.mfglet.2019.08.002>.
- ²³Ali Reza Kamali, 'Eco-Friendly Production of High Quality Low Cost Graphene and Its Application in Lithium Ion Batteries', *Green Chemistry* 18, no. 7 (29 March 2016): 1952–64, <https://doi.org/10.1039/C5GC02455B>.
- ²⁴Saikumar Manchala et al., 'Novel and Highly Efficient Strategy for the Green Synthesis of Soluble Graphene by Aqueous Polyphenol Extracts of Eucalyptus Bark and Its Applications in High-Performance Supercapacitors', *ACS Sustainable Chemistry & Engineering* 7, no. 13 (1 July 2019): 11612–20, <https://doi.org/10.1021/acssuschemeng.9b01506>.
- ²⁵Duy X. Luong et al., 'Gram-Scale Bottom-up Flash Graphene Synthesis', *Nature* 577, no. 7792 (January 2020): 647–51, <https://doi.org/10.1038/s41586-020-1938-0>.
- ²⁶Janire Peña-Bahamonde et al., 'Recent Advances in Graphene-Based Biosensor Technology with Applications in Life Sciences', *Journal of Nanobiotechnology* 16, no. 1 (22 September 2018): 75, <https://doi.org/10.1186/s12951-018-0400-z>.
- ²⁷Brayan Viana Ribeiro et al., 'Biosensors for the Detection of Respiratory Viruses: A Review', *Talanta Open* 2 (1 December 2020): 100007, <https://doi.org/10.1016/j.talo.2020.100007>.
- ²⁸Carly Tymms et al., 'Scalable COVID-19 Detection Enabled by Lab-on-Chip Biosensors', *Cellular and Molecular Bioengineering* 13, no. 4 (1 August 2020): 313–29, <https://doi.org/10.1007/s12195-020-00642-z>.
- ²⁹Jiaoling Huang et al., 'Silver Nanoparticles Coated Graphene Electrochemical Sensor for the Ultrasensitive Analysis of Avian Influenza Virus H7', *Analytica Chimica Acta* 913 (24 March 2016): 7, <https://doi.org/10.1016/j.aca.2016.01.050>.
- ³⁰Ülkü Anik et al., 'Towards the Electrochemical Diagnostic of Influenza Virus: Development of a Graphene–Au Hybrid Nanocomposite Modified Influenza Virus Biosensor Based on Neuramidase Activity', *Analyst* 143, no. 1 (18 December 2017): 150–56, <https://doi.org/10.1039/C7AN01537B>.
- ³¹Murugan Veerapandian, Robert Hunter, and Suresh Neethirajan, 'Dual Immunosensor Based on Methylene Blue-Electroadsorbed Graphene Oxide for Rapid Detection of the Influenza A Virus Antigen', *Talanta* 155 (1 August 2016): 250–57, <https://doi.org/10.1016/j.talanta.2016.04.047>.
- ³²Chunyu Chan et al., 'A Microfluidic Flow-through Chip Integrated with Reduced Graphene Oxide Transistor for Influenza Virus Gene Detection', *Sensors and Actuators B: Chemical* 251 (1 November 2017): 927–33, <https://doi.org/10.1016/j.snb.2017.05.147>.
- ³³Renu Singh, Seongkyeol Hong, and Jaesung Jang, 'Label-Free Detection of Influenza Viruses Using a Reduced Graphene Oxide-Based Electrochemical Immunosensor Integrated with a Microfluidic Platform', *Scientific Reports* 7, no. 1 (15 February 2017): 42771, <https://doi.org/10.1038/srep42771>.
- ³⁴Shalik R. Joshi et al., 'Low Cost Synthesis of Reduced Graphene Oxide Using Biopolymer for Influenza Virus Sensor', *Materials Science and Engineering: C* 108 (1 March 2020): 110465, <https://doi.org/10.1016/j.msec.2019.110465>.
- ³⁵Akanksha Roberts et al., 'Graphene Functionalized Field-Effect Transistors for Ultrasensitive Detection of Japanese Encephalitis and Avian Influenza Virus', *Scientific Reports* 10, no. 1 (3 September 2020): 14546, <https://doi.org/10.1038/s41598-020-71591-w>.

-
- ³⁶Kazuhiko Matsumoto et al., ‘Graphene Field-Effect Transistor for Biosensor’, in *2016 23rd International Workshop on Active-Matrix Flatpanel Displays and Devices (AM-FPD)*, 2016, 45–46, <https://doi.org/10.1109/AM-FPD.2016.7543613>.
- ³⁷Takao Ono et al., ‘Glycan-Functionalized Graphene-FETs toward Selective Detection of Human-Infectious Avian Influenza Virus’, *Japanese Journal of Applied Physics* 56, no. 3 (7 February 2017): 030302, <https://doi.org/10.7567/JJAP.56.030302>.
- ³⁸T. Ono et al., ‘High-Sensitive and Selective Detection of Human-Infectious Influenza Virus Using Biomimetic Graphene Field-Effect Transistor’, in *2018 76th Device Research Conference (DRC)*, 2018, 1–2, <https://doi.org/10.1109/DRC.2018.8442255>.
- ³⁹Y. Chen, C. Chiang, and J. Huang, ‘Wireless Portable Graphene-FET Biosensor for Detecting H 1 N 1 Virus’, 2017, [/paper/Wireless-Portable-Graphene-FET-Biosensor-for-H-1-N-Chen-Chiang/edd3649cfc53aa765de7193fbd4e86aceaa0c433](https://arxiv.org/abs/1708.04433).
- ⁴⁰Seonghwan Jeong et al., ‘Fluorometric Detection of Influenza Viral RNA Using Graphene Oxide’, *Analytical Biochemistry* 561–562 (15 November 2018): 66–69, <https://doi.org/10.1016/j.ab.2018.09.015>.
- ⁴¹Jaewook Lee, Kenshin Takemura, and Enoch Y. Park, ‘Plasmonic/Magnetic Graphene-Based Magnetofluoro-Immunosensing Platform for Virus Detection’, *Sensors and Actuators B: Chemical* 276 (10 December 2018): 254–61, <https://doi.org/10.1016/j.snb.2018.08.124>.
- ⁴²David S. Kinnamon et al., ‘Screen Printed Graphene Oxide Textile Biosensor for Applications in Inexpensive and Wearable Point-of-Exposure Detection of Influenza for At-Risk Populations’, *Journal of the Electrochemical Society* 165, no. 8 (17 April 2018): B3084, <https://doi.org/10.1149/2.0131808jes>.
- ⁴³Singh, Hong, and Jang, ‘Label-Free Detection of Influenza Viruses Using a Reduced Graphene Oxide-Based Electrochemical Immunosensor Integrated with a Microfluidic Platform’.
- ⁴⁴Meng-Qi Fu et al., ‘Supramolecular Fluorogenic Peptide Sensor Array Based on Graphene Oxide for the Differential Sensing of Ebola Virus’, *Chemical Communications* 56, no. 43 (28 May 2020): 5735–38, <https://doi.org/10.1039/C9CC09981F>.
- ⁴⁵Jia Wen et al., ‘Study on Rolling Circle Amplification of Ebola Virus and Fluorescence Detection Based on Graphene Oxide’, *Sensors and Actuators B: Chemical* 227 (1 May 2016): 655–59, <https://doi.org/10.1016/j.snb.2016.01.036>.
- ⁴⁶Arnab Maity et al., ‘Resonance-Frequency Modulation for Rapid, Point-of-Care Ebola-Glycoprotein Diagnosis with a Graphene-Based Field-Effect Biotransistor’, *Analytical Chemistry* 90, no. 24 (18 December 2018): 14230–38, <https://doi.org/10.1021/acs.analchem.8b03226>.
- ⁴⁷Xin Jin et al., ‘A Field Effect Transistor Modified with Reduced Graphene Oxide for Immunodetection of Ebola Virus’, *Microchimica Acta* 186, no. 4 (7 March 2019): 223, <https://doi.org/10.1007/s00604-019-3256-5>.
- ⁴⁸Yantao Chen et al., ‘Field-Effect Transistor Biosensor for Rapid Detection of Ebola Antigen’, *Scientific Reports* 7, no. 1 (8 September 2017): 10974, <https://doi.org/10.1038/s41598-017-11387-7>.
- ⁴⁹Seon-Ah Jin et al., ‘Impedimetric Dengue Biosensor Based on Functionalized Graphene Oxide Wrapped Silica Particles’, *Electrochimica Acta* 194 (10 March 2016): 422–30, <https://doi.org/10.1016/j.electacta.2016.02.116>.
- ⁵⁰Pandiyaraj Kanagavalli and Murugan Veerapandian, ‘Opto-Electrochemical Functionality of Ru(II)-Reinforced Graphene Oxide Nanosheets for Immunosensing of Dengue Virus Non-Structural 1 Protein’, *Biosensors and Bioelectronics* 150 (15 February 2020): 111878, <https://doi.org/10.1016/j.bios.2019.111878>.
- ⁵¹Nur Alia Sheh Omar et al., ‘Sensitive Surface Plasmon Resonance Performance of Cadmium Sulfide Quantum Dots-Amine Functionalized Graphene Oxide Based Thin Film towards Dengue Virus E-Protein’, *Optics & Laser Technology* 114 (1 June 2019): 204–8, <https://doi.org/10.1016/j.optlastec.2019.01.038>.
- ⁵²Nur Alia Sheh Omar et al., ‘Quantitative and Selective Surface Plasmon Resonance Response Based on a Reduced Graphene Oxide–Polyamidoamine Nanocomposite for Detection of Dengue Virus E-Proteins’, *Nanomaterials* 10, no. 3 (March 2020): 569, <https://doi.org/10.3390/nano10030569>.
- ⁵³Nur Alia Sheh Omar et al., ‘Sensitive Detection of Dengue Virus Type 2 E-Proteins Signals Using Self-Assembled Monolayers/Reduced Graphene Oxide-PAMAM Dendrimer Thin Film-SPR Optical Sensor’, *Scientific Reports* 10, no. 1 (11 February 2020): 2374, <https://doi.org/10.1038/s41598-020-59388-3>.
- ⁵⁴Ji-Seon Lee et al., ‘Graphene Oxide-Based Molecular Diagnostic Biosensor for Simultaneous Detection of Zika and Dengue Viruses’, *2D Materials* 7, no. 4 (July 2020): 044001, <https://doi.org/10.1088/2053-1583/ab9a64>.
- ⁵⁵Y. Mustapha Kamil et al., ‘Dengue E Protein Detection Using a Graphene Oxide Integrated Tapered Optical Fiber Sensor’, *IEEE Journal of Selected Topics in Quantum Electronics* 25, no. 1 (January 2019): 1–8, <https://doi.org/10.1109/JSTQE.2018.2846044>.
- ⁵⁶Krongkaew Navakul et al., ‘A Novel Method for Dengue Virus Detection and Antibody Screening Using a Graphene-Polymer Based Electrochemical Biosensor’, *Nanomedicine: Nanotechnology, Biology and Medicine* 13, no. 2 (1 February 2017): 549–57, <https://doi.org/10.1016/j.nano.2016.08.009>.

-
- ⁵⁷Giwan Seo et al., ‘Rapid Detection of COVID-19 Causative Virus (SARS-CoV-2) in Human Nasopharyngeal Swab Specimens Using Field-Effect Transistor-Based Biosensor’, *ACS Nano* 14, no. 4 (28 April 2020): 5135–42, <https://doi.org/10.1021/acsnano.0c02823>.
- ⁵⁸Xiaoyan Zhang et al., ‘Electrical Probing of COVID-19 Spike Protein Receptor Binding Domain via a Graphene Field-Effect Transistor’, *ArXiv:2003.12529 [Cond-Mat, Physics:Physics]*, 27 March 2020, <http://arxiv.org/abs/2003.12529>.
- ⁵⁹Maha Alafeef et al., ‘Rapid, Ultrasensitive, and Quantitative Detection of SARS-CoV-2 Using Antisense Oligonucleotides Directed Electrochemical Biosensor Chip’, *ACS Nano* 14, no. 12 (22 December 2020): 17028–45, <https://doi.org/10.1021/acsnano.0c06392>.
- ⁶⁰Giuseppina Simone, ‘Graphene-Based Optical Sensors for the Pre-Vention of SARS-CoV-2 Viral Dissemination’, *ArXiv:2011.02181 [Physics]*, 4 November 2020, <http://arxiv.org/abs/2011.02181>.
- ⁶¹Hui Zhao et al., ‘Ultrasensitive Supersandwich-Type Electrochemical Sensor for SARS-CoV-2 from the Infected COVID-19 Patients Using a Smartphone’, *Sensors and Actuators B: Chemical* 327 (15 January 2021): 128899, <https://doi.org/10.1016/j.snb.2020.128899>.
- ⁶²Seyyed Alireza Hashemi et al., ‘Ultra-Sensitive Viral Glycoprotein Detection NanoSystem toward Accurate Tracing SARS-CoV-2 in Biological/Non-Biological Media’, *Biosensors and Bioelectronics* 171 (1 January 2021): 112731, <https://doi.org/10.1016/j.bios.2020.112731>.
- ⁶³Rebeca M. Torrente-Rodríguez et al., ‘SARS-CoV-2 RapidPlex: A Graphene-Based Multiplexed Telemedicine Platform for Rapid and Low-Cost COVID-19 Diagnosis and Monitoring’, *Matter* 3, no. 6 (2 December 2020): 1981–98, <https://doi.org/10.1016/j.matt.2020.09.027>.
- ⁶⁴Abdulhadee Yakoh et al., ‘Paper-Based Electrochemical Biosensor for Diagnosing COVID-19: Detection of SARS-CoV-2 Antibodies and Antigen’, *Biosensors and Bioelectronics* 176 (15 March 2021): 112912, <https://doi.org/10.1016/j.bios.2020.112912>.
- ⁶⁵Alireza Samavati et al., ‘Sustainable and Fast Saliva-Based COVID-19 Virus Diagnosis Kit Using a Novel GO-Decorated Au/FBG Sensor’, *Chemical Engineering Journal*, 10 November 2020, 127655, <https://doi.org/10.1016/j.cej.2020.127655>.
- ⁶⁶Md Azahar Ali et al., ‘Sensing of COVID-19 Antibodies in Seconds via Aerosol Jet Nanoprinted Reduced-Graphene-Oxide-Coated 3D Electrodes’, *Advanced Materials* n/a, no. n/a (n.d.): 2006647, <https://doi.org/10.1002/adma.202006647>.
- ⁶⁷Alafeef et al., ‘Rapid, Ultrasensitive, and Quantitative Detection of SARS-CoV-2 Using Antisense Oligonucleotides Directed Electrochemical Biosensor Chip’.
- ⁶⁸Fei Liu et al., ‘Micropatterned Reduced Graphene Oxide Based Field-Effect Transistor for Real-Time Virus Detection’, *Sensors and Actuators B: Chemical* 186 (1 September 2013): 252–57, <https://doi.org/10.1016/j.snb.2013.05.097>.
- ⁶⁹Fei Liu et al., ‘Graphene-Based Electrochemical Biosensor for Pathogenic Virus Detection’, *BioChip Journal* 5, no. 2 (1 June 2011): 123–28, <https://doi.org/10.1007/s13206-011-5204-2>.
- ⁷⁰Mudita Pant et al., ‘Detection of Rota Virus with the Help of Nanomaterial Based Field Effect Transistor (BIO-FET)’, *Biosensors Journal* 6, no. 2 (20 December 2017): 1–7, <https://doi.org/10.4172/2090-4967.1000149>.
- ⁷¹Zhen Fan et al., ‘Accurate Identification and Selective Removal of Rotavirus Using a Plasmonic–Magnetic 3D Graphene Oxide Architecture’, *The Journal of Physical Chemistry Letters* 5, no. 18 (18 September 2014): 3216–21, <https://doi.org/10.1021/jz501402b>.
- ⁷²Jae Hwan Jung, F. Liu, and T. S. Seo, ‘Graphene Oxide-Based Immunobiosensor for Ultrasensitive Pathogen Detection’, in *10th IEEE International Conference on Nanotechnology*, 2010, 692–95, <https://doi.org/10.1109/NANO.2010.5697935>.
- ⁷³Ke-Jing Huang et al., ‘Disposable Immunoassay for Hepatitis B Surface Antigen Based on a Graphene Paste Electrode Functionalized with Gold Nanoparticles and a Nafion–Cysteine Conjugate’, *Microchimica Acta* 177, no. 3 (1 June 2012): 419–26, <https://doi.org/10.1007/s00604-012-0805-6>.
- ⁷⁴Minghuan Liu et al., ‘Graphene Oxide Wrapped with Gold Nanorods as a Tag in a SERS Based Immunoassay for the Hepatitis B Surface Antigen’, *Microchimica Acta* 185, no. 10 (14 September 2018): 458, <https://doi.org/10.1007/s00604-018-2989-x>.
- ⁷⁵Mohamad Farid Abd Muain et al., ‘Gold Nanoparticle-Decorated Reduced-Graphene Oxide Targeting Anti Hepatitis B Virus Core Antigen’, *Bioelectrochemistry* 122 (1 August 2018): 199–205, <https://doi.org/10.1016/j.bioelechem.2018.04.004>.
- ⁷⁶F. Walters et al., ‘Real-Time Detection of Hepatitis B Surface Antigen Using a Hybrid Graphene-Gold Nanoparticle Biosensor’, *2D Materials* 7, no. 2 (March 2020): 024009, <https://doi.org/10.1088/2053-1583/ab734c>.

- ⁷⁷Dheyaa Hussein Mohsin, Muthana Saleh Mashkour, and Fataneh Fatemi, 'Design of Aptamer-Based Sensing Platform Using Gold Nanoparticles Functionalized Reduced Graphene Oxide for Ultrasensitive Detection of Hepatitis B Virus', *Chemical Papers*, 4 August 2020, <https://doi.org/10.1007/s11696-020-01292-1>.
- ⁷⁸Feijun Zhao et al., 'Label-Free Amperometric Immunosensor Based on Graphene Oxide and Ferrocene-Chitosan Nanocomposites for Detection of Hepatitis B Virus Antigen', *Journal of Biomedical Nanotechnology* 13, no. 10 (1 October 2017): 1300–1308, <https://doi.org/10.1166/jbn.2017.2415>.
- ⁷⁹ Feijun Zhao et al., 'An Electrochemical Immunosensor with Graphene-Oxide-Ferrocene-Based Nanocomposites for Hepatitis B Surface Antigen Detection', *Electroanalysis* 30, no. 11 (2018): 2774–80, <https://doi.org/10.1002/elan.201800476>.
- ⁸⁰Qian Xiang et al., 'A Label-Free Electrochemical Platform for the Highly Sensitive Detection of Hepatitis B Virus DNA Using Graphene Quantum Dots', *RSC Advances* 8, no. 4 (2018): 1820–25, <https://doi.org/10.1039/C7RA11945C>.
- ⁸¹Zhaoling Tan et al., 'A Label-Free Immunosensor for the Sensitive Detection of Hepatitis B e Antigen Based on PdCu Tripod Functionalized Porous Graphene Nanoenzymes', *Bioelectrochemistry* 133 (1 June 2020): 107461, <https://doi.org/10.1016/j.bioelechem.2020.107461>.
- ⁸²R. Ray et al., 'Label-Free Biomolecule Detection in Physiological Solutions With Enhanced Sensitivity Using Graphene Nanogrids FET Biosensor', *IEEE Transactions on NanoBioscience* 17, no. 4 (October 2018): 433–42, <https://doi.org/10.1109/TNB.2018.2863734>.
- ⁸³J. Basu and C. Roy Chaudhuri, 'Attomolar Sensitivity of FET Biosensor Based on Smooth and Reliable Graphene Nanogrids', *IEEE Electron Device Letters* 37, no. 4 (April 2016): 492–95, <https://doi.org/10.1109/LED.2016.2526064>.
- ⁸⁴Seongchan Kim et al., 'Deoxyribozyme-Loaded Nano-Graphene Oxide for Simultaneous Sensing and Silencing of the Hepatitis C Virus Gene in Liver Cells', *Chemical Communications* 49, no. 74 (20 August 2013): 8241–43, <https://doi.org/10.1039/C3CC43368D>.
- ⁸⁵Akram Valipour and Mahmoud Roushani, 'Using Silver Nanoparticle and Thiol Graphene Quantum Dots Nanocomposite as a Substratum to Load Antibody for Detection of Hepatitis C Virus Core Antigen: Electrochemical Oxidation of Riboflavin Was Used as Redox Probe', *Biosensors and Bioelectronics* 89 (15 March 2017): 946–51, <https://doi.org/10.1016/j.bios.2016.09.086>.
- ⁸⁶Jialong Fan et al., 'An Ultrasensitive and Simple Assay for the Hepatitis C Virus Using a Reduced Graphene Oxide-Assisted Hybridization Chain Reaction', *Analyst* 144, no. 13 (24 June 2019): 3972–79, <https://doi.org/10.1039/C9AN00179D>.
- ⁸⁷Jingwen Li et al., 'Sensitive Electrochemical Detection of Hepatitis C Virus Subtype Based on Nucleotides Assisted Magnetic Reduced Graphene Oxide-Copper Nano-Composite', *Electrochemistry Communications* 110 (1 January 2020): 106601, <https://doi.org/10.1016/j.elecom.2019.106601>.
- ⁸⁸Ping Jiang et al., 'Ultrasensitive Detection of Hepatitis C Virus DNA Subtypes Based on Cucurbituril and Graphene Oxide Nano-Composite', *Chemical Research in Chinese Universities* 36, no. 2 (1 April 2020): 307–12, <https://doi.org/10.1007/s40242-020-9111-8>.
- ⁸⁹Huayu Huang et al., 'An Ultrasensitive Electrochemical DNA Biosensor Based on Graphene/Au Nanorod/Polythionine for Human Papillomavirus DNA Detection', *Biosensors and Bioelectronics* 68 (15 June 2015): 442–46, <https://doi.org/10.1016/j.bios.2015.01.039>.
- ⁹⁰Fereshteh Chekin et al., 'Nucleic Aptamer Modified Porous Reduced Graphene Oxide/MoS₂ Based Electrodes for Viral Detection: Application to Human Papillomavirus (HPV)', *Sensors and Actuators B: Chemical* 262 (1 June 2018): 991–1000, <https://doi.org/10.1016/j.snb.2018.02.065>.
- ⁹¹Leila Farzin et al., 'Electrochemical Genosensor Based on Carbon Nanotube/Amine-Ionic Liquid Functionalized Reduced Graphene Oxide NanoplatforM for Detection of Human Papillomavirus (HPV16)-Related Head and Neck Cancer', *Journal of Pharmaceutical and Biomedical Analysis* 179 (5 February 2020): 112989, <https://doi.org/10.1016/j.jpba.2019.112989>.
- ⁹²Patrik Aspermaier et al., 'Reduced Graphene Oxide-Based Field Effect Transistors for the Detection of E7 Protein of Human Papillomavirus in Saliva', *Analytical and Bioanalytical Chemistry*, 20 August 2020, <https://doi.org/10.1007/s00216-020-02879-z>.
- ⁹³Pegah Mahmoodi et al., 'Early-Stage Cervical Cancer Diagnosis Based on an Ultra-Sensitive Electrochemical DNA Nanobiosensor for HPV-18 Detection in Real Samples', *Journal of Nanobiotechnology* 18, no. 1 (13 January 2020): 11, <https://doi.org/10.1186/s12951-020-0577-9>.
- ⁹⁴Jaewook Lee et al., 'Binary Nanoparticle Graphene Hybrid Structure-Based Highly Sensitive Biosensing Platform for Norovirus-Like Particle Detection', *ACS Applied Materials & Interfaces* 9, no. 32 (16 August 2017): 27298–304, <https://doi.org/10.1021/acsami.7b07012>.

- ⁹⁵Syed Rahin Ahmed et al., 'Size-Controlled Preparation of Peroxidase-like Graphene-Gold Nanoparticle Hybrids for the Visible Detection of Norovirus-like Particles', *Biosensors and Bioelectronics* 87 (15 January 2017): 558–65, <https://doi.org/10.1016/j.bios.2016.08.101>.
- ⁹⁶Rohit Chand and Suresh Neethirajan, 'Microfluidic Platform Integrated with Graphene-Gold Nano-Composite Aptasensor for One-Step Detection of Norovirus', *Biosensors and Bioelectronics* 98 (15 December 2017): 47–53, <https://doi.org/10.1016/j.bios.2017.06.026>.
- ⁹⁷Ojodomo J. Achadu et al., 'Molybdenum Trioxide Nanocubes Aligned on a Graphene Oxide Substrate for the Detection of Norovirus by Surface-Enhanced Raman Scattering', *ACS Applied Materials & Interfaces* 12, no. 39 (30 September 2020): 43522–34, <https://doi.org/10.1021/acsami.0c14729>.
- ⁹⁸Lichen Xiang et al., 'Inkjet-Printed Flexible Biosensor Based on Graphene Field Effect Transistor', *IEEE Sensors Journal* 16, no. 23 (December 2016): 8359–64, <https://doi.org/10.1109/JSEN.2016.2608719>.
- ⁹⁹Xuan Weng and Suresh Neethirajan, 'Aptamer-Based Fluorometric Determination of Norovirus Using a Paper-Based Microfluidic Device', *Microchimica Acta* 184, no. 11 (1 November 2017): 4545–52, <https://doi.org/10.1007/s00604-017-2467-x>.
- ¹⁰⁰Brian Kim, Kang Wook Chung, and Ji Hoon Lee, 'Non-Stop Aptasensor Capable of Rapidly Monitoring Norovirus in a Sample', *Journal of Pharmaceutical and Biomedical Analysis* 152 (15 April 2018): 315–21, <https://doi.org/10.1016/j.jpba.2018.02.022>.
- ¹⁰¹Chand and Neethirajan, 'Microfluidic Platform Integrated with Graphene-Gold Nano-Composite Aptasensor for One-Step Detection of Norovirus'.
- ¹⁰²Qiaojuan Gong et al., 'A Sensitive Impedimetric DNA Biosensor for the Determination of the HIV Gene Based on Electrochemically Reduced Graphene Oxide', *Analytical Methods* 7, no. 6 (12 March 2015): 2554–62, <https://doi.org/10.1039/C5AY00111K>.
- ¹⁰³Qiaojuan Gong, Yongdong Wang, and Haiying Yang, 'A Sensitive Impedimetric DNA Biosensor for the Determination of the HIV Gene Based on Graphene-Nafion Composite Film', *Biosensors and Bioelectronics*, 2D Materials in Biosensors & Bioelectronics, 89 (15 March 2017): 565–69, <https://doi.org/10.1016/j.bios.2016.02.045>.
- ¹⁰⁴Qiaojuan Gong et al., 'Sensitive Electrochemical DNA Sensor for the Detection of HIV Based on a Polyaniline/Graphene Nanocomposite', *Journal of Materials*, Solid State Ionic Materials, 5, no. 2 (1 June 2019): 313–19, <https://doi.org/10.1016/j.jmat.2019.03.004>.
- ¹⁰⁵Lijun Wang et al., 'A T7exonuclease-Assisted Target Recycling Amplification with Graphene Oxide Acting as the Signal Amplifier for Fluorescence Polarization Detection of Human Immunodeficiency Virus (HIV) DNA', *Luminescence* 31, no. 2 (2016): 573–79, <https://doi.org/10.1002/bio.2997>.
- ¹⁰⁶Oh Seok Kwon et al., 'Large-Scale Graphene Micropattern Nano-Biohybrids: High-Performance Transducers for FET-Type Flexible Fluidic HIV Immunoassays', *Advanced Materials* 25, no. 30 (2013): 4177–85, <https://doi.org/10.1002/adma.201301523>.
- ¹⁰⁷Saurav Islam et al., 'A Smart Nanosensor for the Detection of Human Immunodeficiency Virus and Associated Cardiovascular and Arthritis Diseases Using Functionalized Graphene-Based Transistors', *Biosensors and Bioelectronics* 126 (1 February 2019): 792–99, <https://doi.org/10.1016/j.bios.2018.11.041>.
- ¹⁰⁸Jin Woo Kim et al., 'Attomolar Detection of Virus by Liquid Coplanar-Gate Graphene Transistor on Plastic', *Nanotechnology* 30, no. 34 (May 2019): 345502, <https://doi.org/10.1088/1361-6528/ab0f52>.
- ¹⁰⁹Ramya Vishnubhotla et al., 'Scalable Graphene Aptasensors for Drug Quantification', *AIP Advances* 7, no. 11 (1 November 2017): 115111, <https://doi.org/10.1063/1.4990798>.
- ¹¹⁰Rong Sheng Li et al., 'Boron and Nitrogen Co-Doped Single-Layered Graphene Quantum Dots: A High-Affinity Platform for Visualizing the Dynamic Invasion of HIV DNA into Living Cells through Fluorescence Resonance Energy Transfer', *Journal of Materials Chemistry B* 5, no. 44 (15 November 2017): 8719–24, <https://doi.org/10.1039/C7TB02356A>.
- ¹¹¹Youwen Zhang et al., 'Graphene Oxide-Based Biosensing Platform for Rapid and Sensitive Detection of HIV-1 Protease', *Analytical and Bioanalytical Chemistry* 410, no. 24 (1 September 2018): 6177–85, <https://doi.org/10.1007/s00216-018-1224-2>.
- ¹¹²Anuj Nehra et al., 'Graphene Oxide-Polycarbonate Track-Etched Nanosieve Platform for Sensitive Detection of Human Immunodeficiency Virus Envelope Glycoprotein', *ACS Applied Materials & Interfaces* 9, no. 38 (27 September 2017): 32621–34, <https://doi.org/10.1021/acsami.7b12103>.
- ¹¹³'Ultrasensitive Electrochemical Biosensor for HIV Gene Detection Based on Graphene Stabilized Gold Nanoclusters with Exonuclease Amplification | ACS Applied Materials & Interfaces', accessed 17 January 2021, <https://pubs.acs.org/doi/10.1021/acsami.5b05857>.
- ¹¹⁴Savannah Afsahi et al., 'Novel Graphene-Based Biosensor for Early Detection of Zika Virus Infection', *Biosensors and Bioelectronics* 100 (15 February 2018): 85–88, <https://doi.org/10.1016/j.bios.2017.08.051>.

-
- ¹¹⁵Anna C. R. Moço et al., ‘Electrochemical Detection of Zika Virus in Biological Samples: A Step for Diagnosis Point-of-Care’, *Electroanalysis* 31, no. 8 (2019): 1580–87, <https://doi.org/10.1002/elan.201900068>.
- ¹¹⁶Seon-Ah Jin et al., ‘Impedimetric Zika and Dengue Biosensor Based on Functionalized Graphene Oxide Wrapped Silica Particles’, 1 March 2017, E5.010.
- ¹¹⁷Xiaotong Li et al., ‘An Impedimetric Immunosensor for Determination of Porcine Epidemic Diarrhea Virus Based on the Nanocomposite Consisting of Molybdenum Disulfide/Reduced Graphene Oxide Decorated with Gold Nanoparticles’, *Microchimica Acta* 187, no. 4 (12 March 2020): 217, <https://doi.org/10.1007/s00604-020-4166-2>.
- ¹¹⁸Ankan Dutta Chowdhury et al., ‘Electrical Pulse-Induced Electrochemical Biosensor for Hepatitis E Virus Detection’, *Nature Communications* 10, no. 1 (19 August 2019): 3737, <https://doi.org/10.1038/s41467-019-11644-5>.
- ¹¹⁹G. Czilwik et al., ‘Rapid and Fully Automated Bacterial Pathogen Detection on a Centrifugal-Microfluidic LabDisk Using Highly Sensitive Nested PCR with Integrated Sample Preparation’, *Lab on a Chip* 15, no. 18 (25 August 2015): 3749–59, <https://doi.org/10.1039/C5LC00591D>.
- ¹²⁰Yi Sun et al., ‘A Lab-on-a-Chip System with Integrated Sample Preparation and Loop-Mediated Isothermal Amplification for Rapid and Quantitative Detection of Salmonella Spp. in Food Samples’, *Lab on a Chip* 15, no. 8 (31 March 2015): 1898–1904, <https://doi.org/10.1039/C4LC01459F>.
- ¹²¹Guoliang Huang et al., ‘A Rapid, Low-Cost, and Microfluidic Chip-Based System for Parallel Identification of Multiple Pathogens Related to Clinical Pneumonia’, *Scientific Reports* 7, no. 1 (25 July 2017): 6441, <https://doi.org/10.1038/s41598-017-06739-2>.
- ¹²²Bo Pang et al., ‘Development of a Self-Priming PDMS/Paper Hybrid Microfluidic Chip Using Mixed-Dye-Loaded Loop-Mediated Isothermal Amplification Assay for Multiplex Foodborne Pathogens Detection’, *Analytica Chimica Acta* 1040 (21 December 2018): 81–89, <https://doi.org/10.1016/j.aca.2018.07.024>.
- ¹²³Qingchang Tian et al., ‘An Integrated Temporary Negative Pressure Assisted Microfluidic Chip for DNA Isolation and Digital PCR Detection’, *RSC Advances* 5, no. 100 (25 September 2015): 81889–96, <https://doi.org/10.1039/C5RA18166F>.
- ¹²⁴Stephen J Salipante and Keith R Jerome, ‘Digital PCR—An Emerging Technology with Broad Applications in Microbiology’, *Clinical Chemistry* 66, no. 1 (1 January 2020): 117–23, <https://doi.org/10.1373/clinchem.2019.304048>.
- ¹²⁵Alison Burklund et al., ‘Printable QR Code Paper Microfluidic Colorimetric Assay for Screening Volatile Biomarkers’, *Biosensors and Bioelectronics* 128 (1 March 2019): 97–103, <https://doi.org/10.1016/j.bios.2018.12.026>.
- ¹²⁶Nikhil Bhalla et al., ‘Opportunities and Challenges for Biosensors and Nanoscale Analytical Tools for Pandemics: COVID-19’, *ACS Nano* 14, no. 7 (28 July 2020): 19, <https://doi.org/10.1021/acsnano.0c04421>.