
VISION CONTROLLED SENSORIZED PROSTHETIC HAND

Md Abdul Baset Sarker, Juan Pablo S. Sola, Aaron Jones, Evan Laing, Ernesto Sola-Thomas, Masudul H. Imtiaz

Clarkson University
Potsdam, NY, USA

sarkerm@clarkson.edu, schumaj@clarkson.edu, aarjones@clarkson.edu
lainge@clarkson.edu, schumae@clarkson.edu, mimtiaz@clarkson.edu

ABSTRACT

This paper presents a sensorized vision-enabled prosthetic hand aimed at replicating a natural hand's performance, functionality, appearance, and comfort. The design goal was to create an accessible substitution with a user-friendly interface requiring little to no training. Our mechanical hand uses a camera and embedded processors to perform most of these tasks. The interfaced pressure sensor is used to get pressure feedback and ensure a safe grasp of the object; an accelerometer is used to detect gestures and release the object. Unlike current EMG-based designs, the prototyped hand does not require personalized training. The details of the design, trade-off, results, and informing the next iteration are presented in this paper.

Video: <https://www.youtube.com/watch?v=yInMzI4Ef7A>

Keywords Amputee · AI · Camera · Vision · Prosthetic Hand · Google Coral · 3D print

1 Introduction

By the year 2050, the number of people estimated to be living with the loss of an upper limb is 3.6 million [1]. Since the use of the upper extremities is essential for communication and the performance of day-to-day activities, assistive devices have been developed, modified, and researched to aid impaired individuals. These prosthetics would have the capability to enable people with functional difficulties to lead more productive and dignified lives, participating in education, the labor market, and social life [2]. Prosthetic devices can be classified into two categories: fully actuated and under-actuated. A fully actuated prosthetic more closely replicates the actions and mobility of a natural hand, including up to 27 degrees of freedom: four in each finger, three for extension and flexion, and one for abduction and adduction [2] [3]. An under-actuated prosthetic removes some degrees of freedom to reduce complexity, cost, power consumption, and weight. Most prosthetic hands tend towards under-actuated mechanisms, often by fixing the thumb in place, making it far more difficult for users to grasp a wide range of objects.

Current research has emphasized the implementation of various sensors into the prosthetic hand. Joseph et al. [4] developed a prosthetic hand by placing a camera in the palm to perform real-time grasp selection and implementing a convolutional neural network (CNN) on the NVIDIA Tegra processor. They took images for training from DeepGrasping, ImageNet, and locally captured images. Their design utilized a single-board computer too large to be placed on the hand. Another prosthetic hand using cameras was developed by Shi et al. [5] that can perform "reach-and-pick up" tasks on various daily objects with vision-based myoelectric control. The authors used a 3D camera, Kinect2.0, to capture color (1920×1080) and depth (512 × 424) images at 30 Hz. They placed the camera at a distance from the table, not on the hand itself. A multilayer CNN was used to determine the grasp selection, and an EMG signal was used to control the device. Weiner et al. [6] placed a 1.3-megapixel RGB camera on the palm and an LCD on the black side of their KIT underactuated prosthetic hand. Using two motors, it could provide 10 degrees of freedom. No additional sensors were added to provide an accurate distance measurement; rather, the camera was used to serve this purpose. An ARM Cortex M7 processor (STM32F7) was the main processor.

We also based our design on cameras and deep learning but used more sensors. We added a 5-megapixel camera on the wrist position for vision and five pressure sensors (FSR) on the fingertips to get pressure feedback. A distance sensor was also placed beside the camera to get the accurate distance of the object. Finally, an accelerometer was added inside

the body of the hand, enabling gesture recognition for object release. Our motivation was to introduce a 3D printed mechanical hand that can replicate most of the motions and functions a natural hand can perform, such as grasping various objects, tactile feeling, object recognition, and manipulating objects of various shapes. Multiple sensors were implemented on our prosthetic hand to obtain the functionalities.

The paper is organized as follows. First, the design considerations are presented in Section 2. The prototype description is found in Section 3. The 3D hand-design procedure is explained in Section 4. Section 5 presents a detailed description of the electronic hardware, software, and sensors. The system validation procedure is provided in Section 6. Section 7 discusses the validation results, possible applications, system limitations, and future works. The paper is concluded in Section 8.

2 Design Consideration

Our research aim was to develop a prosthetic hand that would be an accessible substitution requiring little to no training and providing the maximum Degrees of Freedom. It was necessary to have good processing power to run vision-enabled models on an embedded processor while maintaining low power consumption. We chose the Coral Dev Board Mini because it is a compact (64mm X 48mm) low-powered single-board computer. Another consideration was based on study results showing that amputees want to reduce the attention they need to invest to use a prosthetic to grasp an object [6, 7, 8] and the time required for training. EMG signal is widely used in prosthetic devices [9, 10, 11]. The quality of this EMG interface varies due to placement and user conditions [6] and may be ineffective for those with upper-arm disabilities. Our design focuses on using the vision-based solution rather than EMG for primary control. For object detection, our device uses CNN, which is popular among researchers [12, 13, 14, 15, 16, 17, 18, 19, 20, 21]. To perform object detection in the embedded device, we have chosen EfficientDet, a scalable and efficient object detection model [22] that can run on embedded devices like Coral Dev Board Mini [23].

Studies have shown that using an elastic or viscoelastic material on the palm and fingers is beneficial for grasping objects due to their increased surface area upon contact [3]. However, products using these materials tend to be more expensive, making them less accessible to many users. Indeed, prosthetics have always been considered costly due to their maintenance cost. We chose PLA (Polylactic acid) to print the hand to make the device lightweight, strong, and affordable. PLA is lightweight, low-cost, and used in different medical and pharmacological applications for 3D object printing [24].

3 Prototype Description

Figure 1 shows the working prototype of the hand and its major sensors. The main processor and other electronic components are housed inside the forearm. This design includes five FSRs, one camera, and one accelerometer. FSRs are placed on the fingertips to provide tactical feedback

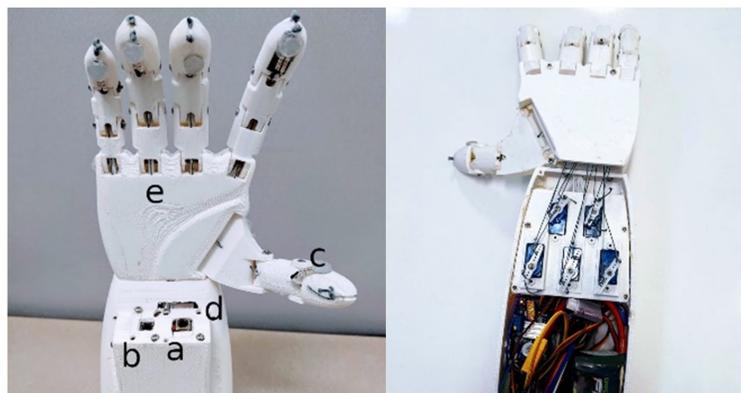


Figure 1: (left) shows the front side of the working prototype of Vision Controlled Sensorized Prosthetic hand: (a) Camera, (b) Distance sensor, (c) Pressure sensor (FSR), (d) accelerometer (hidden inside), (e) Tendon wire. and the image (right) is the backside showing the electronic circuit and servo motor assembly

Each FSR will provide feedback with which the system can determine the force at which an object is being held. The camera is located on the wrist to implement and facilitate automatic object recognition with the help of the proximity

distance sensor. The design and firmware are made open-source (hosted in GitHub [25]) to facilitate mass community adoption. All the sensors described above are interfaced with a single-board computer which collects sensor data from the peripherals and provides control signals to the hand motors to perform the required movements for the prosthetic.

The total length of the designed prosthetic hand after assembly is 373mm, and the size of the palm is “80mm x 86mm x 33.5mm(LxWxD)”. The middle finger length is 88.3mm. The size of the forearm is “205.00mm x 90.50mm x 80mm (LxWxD)”.

4 Mechanical Design

While designing the hand, we considered the system’s strength, reliability, and mobility, as well as the placement and space available for a wide array of sensors and control devices for the hand. The prototype shown below (Figure 2) was printed using Ender 5 3D printer, consuming approximately 289 grams of PLA plastic over around 30 hours. Each finger has its own servo motor. Two tendon wires connect each finger to its servo motor, providing two-directional movement. Our prototype design used the SG90 9G servo, which is robust and readily available.

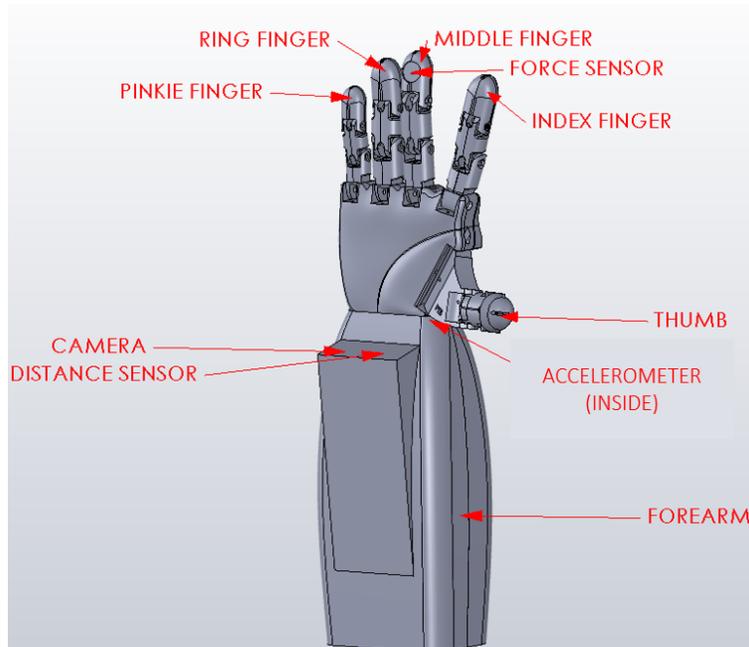


Figure 2: 3D Design of Vision-Enabled Sensorized Prosthetic Hand

5 Electronic Hardware

Figure 3 shows the block diagram of the system, where a MediaTek 8167S (Coral Dev Board Mini) is used as the main processor. A 5MP camera, accelerometer, Time-of-Flight sensor, and a Motor Controller are directly connected to this main processor. A motor controller ATMEGA328P is also connected to the five pressure sensors and servo motors. The pressure sensors are placed on the fingertips of the 3D-printed hand. The camera is connected through the MIPI interface. The accelerometer and TOF sensor are connected to the main processor via an I2C connection. The main processor and ATMEGA328P are connected through UART. Pressure sensors (FSR) are connected to ATMEGA328P using a 10-bit analog-to-digital converter (ADC). Finally, the servo motors are controlled over a PWM signal from five digital I/O pins of ATMEGA328P. We used 11.1v lithium-ion battery with a buck converter that converts 5v to run the devices.

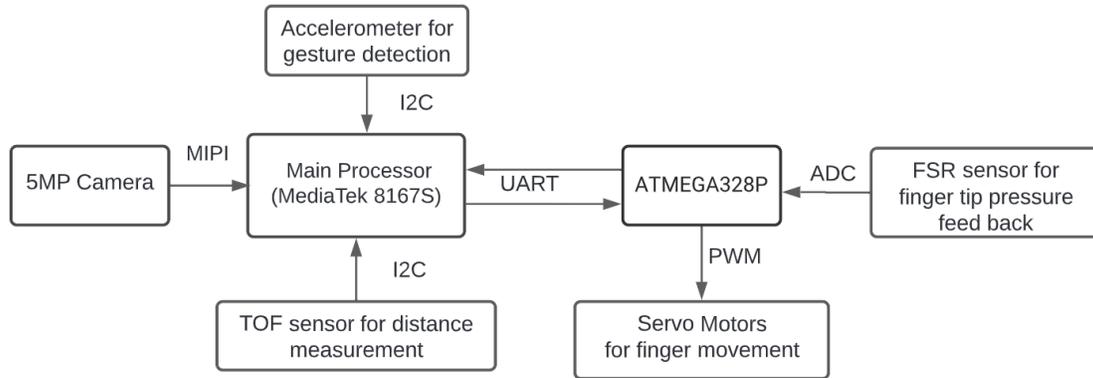


Figure 3: Block diagram of the system

5.1 Coral dev board mini

Coral Dev Board Mini is a low-cost single-board computer. The small version provides fast machine learning (ML) inference [23]. The USB-C-powered Coral Dev Board Mini has a CPU (MediaTek 8167S), GPU (IMG PowerVR GE8300), 2 GB LPDDR3 RAM, 8 GB eMMC flash memory, and more. It has wireless connectivity like Bluetooth and Wi-Fi on board [23]. It also includes an Edge Tensor Processor Unit (TPU) [26]. The Edge TPU has outperformed similar form factor devices' for both latency and computational efficiency [27, 28]. The performance increases dramatically when Edge TPU is included compared to non-Edge TPU devices [28]. Furthermore, it provides good performance with low power consumption [29]. With Coral Dev Board Mini, TensorFlow Lite models can be compiled and run on the Edge TPU. We installed the Mendel Operating system in the internal 8GB flash memory of the Coral Dev Board Mini. A Python script was developed to run continuously upon startup and complete the following tasks:

- Upon object detection, an accurate distance is calculated using the TOF sensor (VL6180x).
- If the object is near to the hand, about (70-90mm), it sends a signal “Hand Close” to the motor controller to close the hand.
- While the hand is closing, it gets feedback from the pressure sensors. If the pressure value exceeds a predefined value, it will stop closing the hand.
- Once the hand has closed, the accelerometer (ADXL345) is activated and waits to detect a certain gesture. Upon sensing the gesture, it will send the “Hand Open” signal to the motor controller.

5.2 Camera and Sensors

A 5-megapixel camera module (25mm x 25mm) compatible with Coral boards is used to capture the images. The camera connects through the MIPI-CSI interface and provides an easy way to bring visual input into the model. The camera has autofocus with a focal length of 2.5mm and a range of 10cm to infinity. The camera's view angle is 84/87 degrees, and it has auto white balance control, auto exposure control, auto band filter, auto black level calibration, and auto 50/60Hz illumination that helps get optimized images for object detection [30]. Some researchers placed the camera inside the thumb [6]. we decided to place the camera on the wrist to reduce interference from the fingers. Five Force Sensitive Resistors (FSRs) are attached to each fingertip of the prosthetic to get pressure feedback for the hand while grasping the object. When the “Hand Close” command is initiated, the motor controller starts to close the hand by controlling servo motors by sensing the pressure from FSR. The VL6180X is a Time of Flight distance sensor that contains a very tiny laser source and a matching sensor. The VL6180X can detect the Time of Flight for the laser to bounce back to the sensor; VL6180X uses a very narrow light source to determine the distance of the surface directly in front of it. The VL6180X is much more precise and doesn't have linearity or 'double imaging' problems compared to other solutions [31]. VL6180X is used here to detect the exact distance of the object from the hand. When an object is detected by the main camera, VL6180X is activated and calculates the object's distance. The main processor sends a signal to close the hand if the object is between 70-90mm away. The ADXL345 is a low-power, 3-axis MEMS (MicroElectro-Mechanical Systems) accelerometer module. The MEMS dimension can range from several millimeters to less than one micrometer. The MEMS consists of a micro-machined structure on a silicon wafer suspended by polysilicon springs that allow it to deflect smoothly on the X, Y, or Z-axis [32]. Between the plates, the deflection causes a measurable change in capacitance. [33]. ADXL345 is a triple-axis accelerometer with a Digital I2C

and SPI interface breakout. There is an onboard 3.3V regulator and logic-level shifting, so it is easy to interface with a 3V or 5V microcontroller. The sensitivity level can be set to either +2g, +4g, +8g, or +16g, where the lower range gives more resolution for slow movements, and the higher range is good for high-speed tracking. ADXL345 is used in our prosthetic hand to detect a gesture (tilt) to release the object.

5.3 Motor Controller and Motors

ATMEGA328P microcontroller is used as the motor controller. Atmega328p is an 8-bit RSC-based microcontroller that combines 32KB flash memory, 1024B EEPROM, 2KB RAM, 32 I/O pins, 6-channel 10-bit A/D converter, UART, SPI, etc. [34]. The ATMEGA328P is connected to the main processor through serial communication that accepts the signals “Hand Close” and “Hand Open.” Five SG90 micro servo motors manipulate the hand via tendon wires.

5.4 Training and object detection

As the Coral Dev Board Mini has a TPU (Tensor Processing Unit) [35], we have used the EfficientDet-Lite0 model architecture [23], [36]. For training, we collected numerous images of two objects. We annotated all the images using the open-source LabelImg script [37]. Then augmented the images and separated 10% used for testing, 10% for validation, and 80% for training.

6 System Validation

As it is a vision-controlled device, our first target was to get real-time object detection. The device was trained and tested with the custom objects. For testing, two objects of different colors were trained and tested with the grasp, lift, and drop functionality several times. These actions were repeated in various locations and lighting conditions. A video was published on YouTube to demonstrate the working of the Vision-Enabled Prosthetic Hand [38]. We ran the test 20 times and got 90% accuracy. As this is a battery-operated device, one of the key requirements is to ensure that a universal and commercially available battery charging system can provide the required current [39]. In this project, we have used one 1300mAh Lithium-Polymer battery. A commercially available lithium polymer charger is used to charge the battery. Any 11.1v charger can charge these batteries. Under lab conditions, this device ran up to one hour under constant use with a single charge.

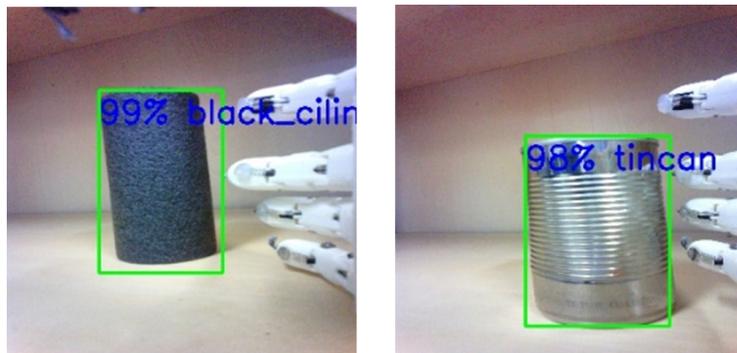


Figure 4: Object detected when the hand is closer to the object



Figure 5: Grasping the object with the prosthetic hand

7 Discussion

In this study, we designed a prosthetic hand with increased functionality, lower weight, and adequate application of force to grasp an object. One of our primary design goals was to reduce the weight and cost, which led to the decision to 3D print the hand using low-cost, durable, and lightweight PLA material. The total weight of the prosthetic hand, including the motor, battery, electronics, and structure, was 413g. For object detection, EfficientDet was used in a Coral Dev Board Mini. The image was captured using a 5MP Coral camera and resized to 320X320 pixels. The pre-trained weights were loaded into the device's flash memory and performed continuously at 9 FPS. Figure 4 shows the object detection when the object is close to the hand. It shows that the tin can and the black cylinder is detected by the hand, and it's ready to grasp the object.

The battery voltage is 11.1v. While idle, the whole system draws 130 mA current. Running the inference takes around 250mA current, and while in operation (object detection and grasping an object), it draws 450mA. The prototype performed basic hand movements, including grasping an object, lifting it, and placing it back down. Figure 5 shows the object grasping in action with the prosthetic hand. This new research area has the potential to revolutionize controlled prosthetic devices, as the deployment of a vision-controlled system provides a global solution for a much larger number of users than the personalized training methods employed using EMG and EEG-based prosthetics. For EMG and EEG-based prosthetics, the training time necessary for the user to operate the prosthetic effectively and to train the model to detect the signal correctly can be extensive. This includes both the user becoming comfortable with the system, including any fitting adjustments, the training of machine learning models, and so on. Naturally, the training time of the device must be compared against the performance of that device once trained. Our prosthetic hand design maintains an access control strategy while maintaining the benefits of a capable, fully actuated prosthetic.

8 Conclusion

The number of people afflicted by the loss of an upper limb is already over 3.6 million and is expected to only grow in the coming years. This market, already worth over \$6 billion, is characterized by expensive, hard to use, and inaccessible products. Furthermore, losing this kind of mobility is devastating to a patient's independence; regaining this independence can be empowering. Our project with the new camera-based control system brings the sophistication of traditional prosthetics into the mainstream market. This new control system requires far less training time than those used by conventional prosthetics, with the potential also to be far more reliable. This is a proof of concept. The next step is to develop a method to attach the hand so that it can be fitted for different ages, sizes, and lengths of the lower arm. Our unique combination of features brings hope to amputees to regain a fully functional hand.

References

- [1] World Health Organization. Seventy-first world health assembly adopts resolution on assistive technology. Available: <https://www.who.int/news/item/15-05-2018-seventy-first-world-health-assembly-adopts-resolution-on-assistive-technology>. Accessed: May 20, 2022.
- [2] MDPI. Applied sciences | free full-text | anthropomorphic prosthetic hand with combination of light weight and diversiform motions | html. Available: <https://www.mdpi.com/2076-3417/9/20/4203/htm>. Accessed: May 20, 2022.
- [3] A. Khurshid, A. Ghafoor, and M. A. Malik. *Robotic Grasping and Fine Manipulation Using Soft Fingertip*. IntechOpen, 2011.
- [4] J. DeGol, A. Akhtar, B. Manja, and T. Bretl. Automatic grasp selection using a camera in a hand prosthesis. In *2016 38th Annual International Conference of the IEEE Engineering in Medicine and Biology Society (EMBC)*, pages 431–434, 2016.
- [5] C. Shi, D. Yang, J. Zhao, and H. Liu. Computer vision-based grasp pattern recognition with application to myoelectric control of dexterous hand prosthesis. *IEEE Transactions on Neural Systems and Rehabilitation Engineering*, 28(9):2090–2099, September 2020.
- [6] P. Weiner, J. Starke, F. Hundhausen, J. Beil, and T. Asfour. The kit prosthetic hand: Design and control. In *2018 IEEE/RSJ International Conference on Intelligent Robots and Systems (IROS)*, pages 3328–3334, 2018.
- [7] C. Pylatiuk, S. Schulz, and L. Döderlein. Results of an internet survey of myoelectric prosthetic hand users. *Prosthetics and Orthotics International*, 31(4):362–370, December 2007.
- [8] F. Cordella and et al. Literature review on needs of upper limb prosthesis users. *Frontiers in Neuroscience*, 10, 2016. Accessed: Jun. 25, 2022.

- [9] K. Akazawa, R. Okuno, and M. Yoshida. Biomimetic emg-prosthesis-hand. In *Proceedings of 18th Annual International Conference of the IEEE Engineering in Medicine and Biology Society*, volume 2, pages 535–536, 1996.
- [10] D. Graupe and W. K. Cline. Functional separation of emg signals via arma identification methods for prosthesis control purposes. *IEEE Transactions on Systems, Man, and Cybernetics*, SMC-5(2):252–259, March 1975.
- [11] C. Cipriani, F. Zacccone, S. Micera, and M. C. Carrozza. On the shared control of an emg-controlled prosthetic hand: Analysis of user–prosthesis interaction. *IEEE Transactions on Robotics*, 24(1):170–184, February 2008.
- [12] W. Li, K. Liu, L. Yan, F. Cheng, Y. Lv, and L. Zhang. Frd-cnn: Object detection based on small-scale convolutional neural networks and feature reuse. *Scientific Reports*, 9(1):10781–10790, November 2019.
- [13] J. Wei, J. He, Y. Zhou, K. Chen, Z. Tang, and Z. Xiong. Enhanced object detection with deep convolutional neural networks for advanced driving assistance. *IEEE Transactions on Intelligent Transportation Systems*, 21(4):1572–1583, April 2020.
- [14] G. Cheng, J. Han, P. Zhou, and D. Xu. Learning rotation-invariant and fisher discriminative convolutional neural networks for object detection. *IEEE Transactions on Image Processing*, 28(1):265–278, January 2019.
- [15] N. V. Kousik, Y. Natarajan, R. A. Raja, S. Kallam, R. Patan, and A. H. Gandomi. Improved salient object detection using hybrid convolution recurrent neural network. *Expert Systems with Applications*, 166:114064, March 2021.
- [16] J. Du. Understanding of object detection based on cnn family and yolo. In *Journal of Physics: Conference Series*, volume 1004, page 012029, April 2018.
- [17] Y. Pi, N. D. Nath, and A. H. Behzadan. Convolutional neural networks for object detection in aerial imagery for disaster response and recovery. *Advanced Engineering Informatics*, 43:101009, January 2020.
- [18] J. Li and et al. Attentive contexts for object detection. *IEEE Transactions on Multimedia*, 19(5):944–954, May 2017.
- [19] S. Tripathi, G. Dane, B. Kang, V. Bhaskaran, and T. Nguyen. Lcdet: Low-complexity fully-convolutional neural networks for object detection in embedded systems. In *CVPR Workshops*, pages 94–103, 2017. Accessed: Jun. 25, 2022.
- [20] Y. Gong and et al. Context-aware convolutional neural network for object detection in vhr remote sensing imagery. *IEEE Transactions on Geoscience and Remote Sensing*, 58(1):34–44, January 2020.
- [21] X. Li and S. Wang. Object detection using convolutional neural networks in a coarse-to-fine manner. *IEEE Geoscience and Remote Sensing Letters*, 14(11):2037–2041, November 2017.
- [22] M. Tan, R. Pang, and Q. V. Le. Efficientdet: Scalable and efficient object detection. In *CVPR*, pages 10781–10790, 2020. Accessed: Jun. 25, 2022.
- [23] Coral. Dev board mini. Available: <https://coral.ai/products/dev-board-mini/>. Accessed: May 19, 2022.
- [24] P. Maróti, B. Kocsis, A. Ferencz, M. Nyitrai, and D. Lőrinczy. Differential thermal analysis of the antibacterial effect of pla-based materials planned for 3d printing. *Journal of Thermal Analysis and Calorimetry*, 139(1):367–374, January 2020.
- [25] M. A. B. Sarker. Vision enabled prosthetic hand. Available: https://github.com/baset-sarker/vision_enabled_prosthetic_hand. Accessed: Jul. 10, 2022.
- [26] S. Cass. Taking ai to the edge: Google’s tpu now comes in a maker-friendly package. *IEEE Spectrum*, 56(5):16–17, May 2019.
- [27] K. Park and et al. Real-time mask detection on google edge tpu. *arXiv*, October 2020.
- [28] J. Sengupta, R. Kubendran, E. Neftci, and A. Andreou. High-speed, real-time, spike-based object tracking and path prediction on google edge tpu. In *2020 2nd IEEE International Conference on Artificial Intelligence Circuits and Systems (AICAS)*, pages 134–135, August 2020.
- [29] S. Hosseininoorbin, S. Layeghy, B. Kusy, R. Jurdak, and M. Portmann. Scaling spectrogram data representation for deep learning on edge tpu. In *2021 IEEE International Conference on Pervasive Computing and Communications Workshops and other Affiliated Events (PerCom Workshops)*, pages 572–578, March 2021.
- [30] Coral. Camera. Available: <https://coral.ai/products/camera>. Accessed: May 20, 2022.
- [31] A. Industries. Adafruit vl6180x time of flight distance ranging sensor (vl6180). Available: <https://www.adafruit.com/product/3316>. Accessed: May 28, 2022.
- [32] Adafruit Learning System. Adxl345 digital accelerometer. Available: <https://learn.adafruit.com/adxl345-digital-accelerometer/overview>. Accessed: May 28, 2022.

- [33] Wikipedia. Microelectromechanical systems, March 2022. Accessed: May 28, 2022.
- [34] Microchip Technology. Atmega328p | microchip technology. Available: <https://www.microchip.com/en-us/product/ATmega328P>. Accessed: May 20, 2022.
- [35] Coral. Coral. Available: <https://coral.ai/>. Accessed: Mar. 29, 2022.
- [36] Brain AutoML. Brain automl, June 2022. Accessed: Jul. 01, 2022.
- [37] darrenl. Labelimg. Available: <https://github.com/tzutalin/labelImg>, June 2022. Accessed: Jun. 29, 2022.
- [38] Vision controlled sensorized prosthetic hand. Available: <https://www.youtube.com/watch?v=7qkj1d9e5f4>, June 2022. Accessed: Jun. 29, 2022.
- [39] M. H. Imtiaz, V. Y. Senyurek, P. Belsare, K. Nagaraja, and E. Sazonov. Development of a smart iot charger for wearable cigarette smoking monitor. In *2019 SoutheastCon*, pages 1–5, April 2019.