## 10<sup>-15</sup>-level laser stabilization down to fiber thermal noise limit using balanced photodetection

IGJU JEON, CHANGMIN AHN, AND JUNGWON KIM\*

Korea Advanced Institute of Science and Technology (KAIST), Daejeon 34141, Republic of Korea \*jungwon.kim@kaist.ac.kr

We demonstrate a self-homodyne detection method to stabilize a continuous-wave 1550-nm laser to a 1-km optical fiber delay line, achieving a frequency instability of  $6.3 \times 10^{-15}$  at a 16-ms averaging time. This result, limited by fiber thermal noise, is achieved without the need for a vacuum system, highlighting the potential of our approach for ultra-stable laser systems in non-laboratory environments. The system utilizes only a few passive fiber optic components and a single balanced photodetector, significantly simplifying the laser stabilization process while maintaining high performance. The entire optical setup is compactly packaged in a portable metal air-tight enclosure.

There is an increasing demand for ultra-stable laser sources that can be used in non-laboratory environments such as atmospheric and gas sensing [1,2], transportable lattice clock [3,4], and earthquake (moonquake) detection [5–7]. Ultra-stable optical frequency comb sources operating outside laboratories can be also utilized in field-deployed dual-comb spectroscopy [8,9] and generation of low-noise microwave [10,11]. To achieve an ultralow-noise laser system, the free-running laser needs to be stabilized to a mechanical length reference using a suitable frequency discrimination system, where both the reference and discriminator should be compact and robust against external mechanical disturbances.


Recent compact laser stabilization approaches focus on smallsized optical cavities with ultra-high Q factors and low thermal noise. Examples include ultra-low expansion (ULE) Fabry-Pérot cavities, dielectric whispering-gallery-mode (WGM) resonators, integrated chip-scale resonators, and optical fiber delay-lines. For instance, vacuum-gap Fabry-Pérot [12–14] and air-gap cavities [15,16] have achieved frequency instabilities of  $10^{-14}$  to  $10^{-15}$ , though they require free-space alignment. Dielectric-WGM resonators [17] or microrod-based systems [18] have achieved stability levels ranging from  $10^{-14}$  to  $10^{-13}$ , which are limited by the thermal noise of the reference. Integrated chip-scale resonators, despite achieving  $10^{-13}$  stabilization, face limitations due to higher thermal noise limit and frequency drift [19].

These systems often rely on the Pound-Drever-Hall (PDH) method [20], which involves optical modulators and many RF components. An alternative is fiber-based systems, such as

stimulated Brillouin scattering (SBS), which can achieve  $10^{-13}$  instability using only 2-m fiber coil [21,22]. Although the SBS process itself does not require the PDH system due to its passive nature, practically, the PDH method is needed to tune the pump laser frequency to the cavity resonance.

Longer optical fiber delays, using self-heterodyne interferometers [23–28] or ring-resonator configurations [29], offer a compact, alignment-free solution. These can stabilize both CW lasers [23,27-29] and optical frequency combs [24-26], achieving high performance with simpler setups. The self-heterodyne systems using kilometers of fiber delay have demonstrated remarkable stability, with sub-Hz linewidths and frequency instabilities as low as 3.2×10<sup>-15</sup> at 1 second [28]. However, achieving these results demands complex setups, including thermal shielding and vacuum systems, which increase the overall system size and complexity. Furthermore, advances in fiber optic coil winding have enabled compact fiber spools, yet in self-heterodyne configurations, components like acousto-optic frequency shifter still limit system miniaturization [26]. Alternatively, a recent solution involves an all-passive ring-resonator with 100-meter polarization-maintaining (PM) fiber, which has achieved a Q factor of 4 billion and 10<sup>-14</sup>-level frequency instability within 0.1 seconds [29]. This design effectively suppresses intensity noise but requires all-PM fiber components and careful management of cavity loss to maintain a high Q factor.

In this Letter, we adopt a non-PM all-single-mode fiber selfhomodyne interferometric configuration with a 1-km vibrationinsensitive optical fiber spool to stabilize CW lasers. Unlike selfheterodyne interferometers, which require acousto-optic modulators and additional RF components, this system uses only a few passive optical components and a single balanced photodetector (BPD) to generate the error signal. The 1-km fiber delay with the Michelson interferometer offers a Q factor of 4 billion. A simple BPD can effectively suppress the coupling of intensity noise of the laser to be stabilized to the frequency noise. We stabilized CW lasers to a 10<sup>-15</sup>-level frequency instability, where the frequency noise is limited by fiber thermal noise in the 4 Hz to 200 Hz range.

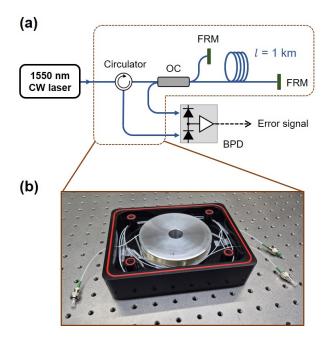

**Fig. 1** (a) configuration of the all-fiber self-homodyne Michelson interferometer with balanced photodetector. OC, optical coupler, FRM, Faraday rotating mirror; BPD, Balanced photodetector. (b) Packaging of the self-homodyne Michelson interferometer with vibration-insensitive 1-km optical fiber spool. The dimension of the case (with lid) is 140×180×51 mm<sup>3</sup>. The photograph does not include the 10-mm thick lid.

The fiber-delay-based Michelson interferometer is composed of four main components: a fiber-coupled circulator, a balanced optical fiber coupler, an optical fiber delay, and two fiber-coupled Faraday rotating mirrors, as shown in Fig. 1(a). We used two Faraday rotating mirrors at the end of the interferometer arms instead of standard fiber-coupled mirrors to match the polarization state between the two interfering signals, maximizing the signal-tonoise ratio (SNR) of the interference signal. To suppress voltage signal fluctuations caused by laser intensity noise, the two interfering optical signals are subtracted using balanced photodetection. One signal comes directly from the coupler, while the other comes from the circulator.

Unlike other platforms where resonators with ultra-high Q factors have narrow dips separated by the free spectral range (FSR), this configuration consistently features a spectral width equal to half of the FSR, with a simple sine-wave-shaped transmittance along the frequency of the laser. Since the FSR is c/nl where c is the speed of light, n is the refractive index of the fiber, and l is the effective length of the fiber delay, the spectral width of the configuration is c/2nl. Note that since we used a Michelson interferometer instead of a Mach-Zehnder interferometer, the effective length of the reference is twice the actual length of the fiber spool we used.


The Q factor of the configuration can be computed as  $4 \times 10^9$  by dividing the optical carrier frequency (193.5 THz at 1550 nm wavelength) by the spectral width. This configuration allows us to achieve an ultra-high Q factor, which can effectively discriminate laser frequency noise. Compared to previous research on all-fiber ring-resonator configurations [29], this setup does not require PM fiber components. Additionally, the Q factor of the system is

maintained regardless of losses inside the cavity.


We packaged the self-homodyne Michelson interferometer, based on a vibration-insensitive 1-km optical fiber spool, in a compact metal enclosure. As shown in Fig. 1(b), the setup uses off-the-shelf optical components arranged as in Fig. 1(a) and includes an optical fiber spool within an air-tight aluminum case measuring  $140 \times 180 \times 51$  mm<sup>3</sup>. The case has an input for the laser signal that needs stabilization and two optical outputs for balancing. To achieve air-tight packaging, we used rubber seals and screws, effectively preventing acoustic noise from compromising the stability of the fiber reference. The packaged setup was used in the stabilization experiments described later.

Figure 2 shows the schematic of the laser stabilization and performance measurement setup. Two 1550 nm diode lasers (ULN15PT and ULN15TK, Thorlabs Inc.) are used as CW laser sources. Approximately 1 mW of optical power from each laser is directed into independent frequency discriminators, each configured as shown in Fig. 1(b), which include a self-homodyne interferometer using a 1-km optical fiber spool. The 1-km optical fiber spool, serving as a mechanical length reference, is designed to be vibration-insensitive as described in Ref [29]. The spool, with dimensions of 100 mm in diameter and 20 mm in height. demonstrates a vibration sensitivity of approximately  $10^{-10}$  [1/g]. The voltage signal detected from the BPD is fed back to the current modulator after passing through PI servos. The two separately stabilized CW lasers produce a beat note frequency of approximately 78.9 MHz. The frequency noise power spectral density was measured using a phase noise analyzer (53100A, Microsemi), and the frequency instability was calculated as the overlapping Allan deviation for averaging times greater than 0.001 seconds.

Figure 3(a) shows the frequency noise spectra for the CW lasers. When the laser is stabilized using the packaged system shown in Fig. 1(b), the frequency noise is reduced by up to  $10^4$  times in the

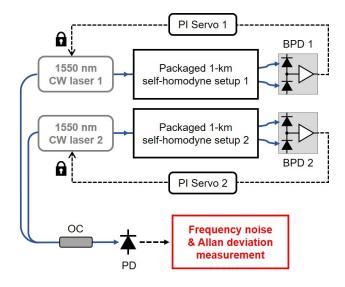

**Fig. 2** Schematic of the laser stabilization and noise measurement setup. Two 1550 nm fiber CW lasers are stabilized using separate all-fiber self-homodyne interferometers. The frequency noise and Allan deviation are then measured by analyzing the beat frequency between the two stabilized lasers.

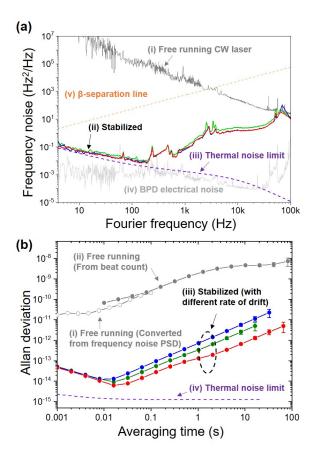


**Fig. 3** Frequency noise spectra and Allan deviation as results of CW lasers stabilization. (a) The frequency noise spectra. (i) freerunning; (ii) stabilized; (iii) thermal-noise limit, which is the summantion of thermomechanical and thermo-refractive fiber noise [30]; and (iv) measured BPD electrical noise. (b) Optical frequency instability in terms of overlapping Allan deviation. (i) free-running frequency instability converted from frequency noise PSD (curve (i) in Fig. 4(a)); (ii) free-running frequency instability calculated from long-term beat measurement; (iii) overlapping Allan deviation of the stabilized CW lasers calculated from beat frequency time trace; and (iv) Thermal noise limit.

Fourier frequency range from 4 Hz to 10 kHz [curves (ii) in Fig. 3(a)] compared to the free-running CW laser [curve (i) in Fig. 3(a)]. The red, green, and blue curves represent different measurement trials, all of which demonstrate similar short-term frequency noise performance. Notably, during short-term noise measurements across all trials, the frequency noise level reaches the thermal noise limit [30,31] of the 1-km fiber round-trip (thus, 2-km effective length) in the 4-200 Hz Fourier frequency range, suggesting that an air-tight casing is sufficient to achieve the lowest frequency noise level without needing a vacuum system. The locking bandwidth in the Michelson interferometer with a 1-km fiber delay is limited to 100 kHz, which accounts for the prominent peak near 100 kHz in Fig. 3(a). Curve (iv) shows the BPD electrical noise, converted from the voltage noise measured from the in-loop BPD output after removing the 1-km spool from the long arm of the interferometer. The fact that this noise level is lower than the thermal noise of the round-trip of the 1-km optical fiber spool indicates that selfhomodyne balanced detection is sufficient to stabilize the laser to the thermal-noise limit of a 2-km fiber. The  $\beta$ -separation line is well above the stabilized laser's frequency noise level, indicating that the linewidth within 0.1 seconds is less than 1 Hz. (The integrated linewidth from a 1 Hz Fourier frequency is calculated as 12 Hz, which is relatively large due to longer-term thermal drift.)

Figure 3(b) illustrates the Allan deviation of the frequency instability. The frequency instability reaches a minimum of 6.3×10<sup>-15</sup> at a 16-ms averaging time with minimal drift. The red, blue, and green curves represent the frequency instabilities corresponding to the trials shown in Fig. 3(a) with the same colors, demonstrating that although all trials produce similar short-term frequency noise PSD, the Allan deviation can differ based on the rate of fiber length drift. For each trial, the drift rates are 28 Hz/s, 120 Hz/s, and 270 Hz/s for the red, green, and blue curves, respectively, as shown in curve (iii) of Fig. 3(b).

Here we present a comparison of our work's performance with other recent non-vacuum compact CW laser stabilization platform results, as shown in Figure 4. Our work is compared with results from stabilization using vacuum-gap Fabry-Pérot cavities operated in air [14], air-gap compact Fabry-Pérot cavities [16], WGM resonators [18], integrated chip-scale resonators [19], and optical

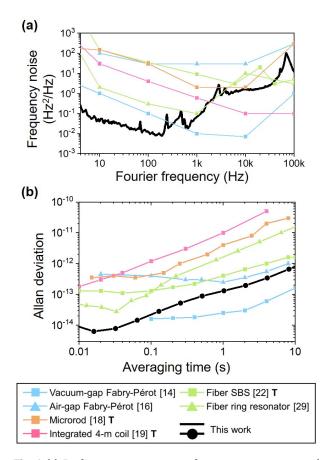

**Fig. 4** (a) Performance comparison of various non-vacuum and compact CW laser stabilization methods including our work. (a) Frequency noise spectrum. (b) Allan deviation. The capital T symbols in the legend indicate the setup is actively temperature-controlled.

fiber delay lines [22,29]. As shown in Fig. 4, our frequency noise and Allan deviation are superior in the 4-100 Hz offset frequency or 10-100 ms averaging time range among other non-vacuum platforms. Achieving 10<sup>-15</sup>-level frequency instability with Fabry-Pérot cavities requires a vacuum and temperature control system, as noted in Refs [12,13]. These systems also require free-space coupling, which can be sensitive to external vibrations or impacts. Microrod and integrated chip resonators require sensitive and vulnerable tapered-fiber or butt coupling, making them difficult to use in harsh environments. Except for the fiber ring resonator configuration, all other platforms require the PDH method, which necessitates additional active optical components and RF components such as VCOs.

In summary, we have demonstrated a super-simple, compact, and alignment-free laser stabilization module based on an all-fiber self-homodyne interferometer using a 1-km optical fiber delay and balanced photodetection. The optical frequency noise of a 1550-nm CW laser was stabilized to the thermal noise limit of the fiber delay. This resulted in minimum frequency instabilities of  $6.3 \times 10^{-15}$  at 16-ms averaging time. This stabilization system requires only an airtight environment to achieve thermal noise-limited performance. The optical part of stabilization system is packaged in a compact aluminum case with dimension of  $140 \times 180 \times 51$  mm<sup>3</sup>, including vibration-insensitive 1-km fiber spool, which makes it highly suitable for field applications outside a laboratory environment.

**Funding.** National Research Foundation (NRF) of Korea (RS-2024-00334727 and 2021R1A5A1032937), National Research Council of Science and Technology (NST) of Korea (CAP22061-000), Institute for Information and Communications Technology Promotion (IITP) of Korea (RS-2023-00223497)

Disclosures. The authors declare no conflicts of interest.

**Data availability.** Data underlying the results presented in this paper are not publicly available at this time but may be obtained from the authors upon reasonable request.

## References

- Y. He, Y. Ma, Y. Tong, X. Yu, and F. K. Tittel, "A portable gas sensor for sensitive CO detection based on quartz-enhanced photoacoustic spectroscopy," Optics & Laser Technology 115, 129–133 (2019).
- M. Mazur, N. K. Fontaine, M. Kelleher, V. Kamalov, R. Ryf, L. Dallachiesa, H. Chen, and D. T. Neilson, "Advanced Distributed Submarine Cable Monitoring and Environmental Sensing using Constant Power Probe Signals and Coherent Detection," arXiv preprint arXiv:2303.06528 (2023).
- J. Grotti, S. Koller, S. Vogt, S. Häfner, U. Sterr, C. Lisdat, H. Denker, C. Voigt, L. Timmen, A. Rolland, F. N. Baynes, H. S. Margolis, M. Zampaolo, P. Thoumany, M. Pizzocaro, B. Rauf, F. Bregolin, A. Tampellini, P. Barbieri, M. Zucco, G. A. Costanzo, C. Clivati, F. Levi, and D. Calonico, "Geodesy and metrology with a transportable optical clock," Nature Phys 14(5), 437–441 (2018).
- M. Takamoto, Y. Tanaka, and H. Katori, "A perspective on the future of transportable optical lattice clocks," Applied Physics Letters 120(14), 140502 (2022).
- G. Marra, C. Clivati, R. Luckett, A. Tampellini, J. Kronjäger, L. Wright, A. Mura, F. Levi, S. Robinson, A. Xuereb, B. Baptie, and D. Calonico, "Ultrastable laser interferometry for earthquake detection with terrestrial and submarine cables," Science **361**(6401), 486–490 (2018).

- G. Marra, D. M. Fairweather, V. Kamalov, P. Gaynor, M. Cantono, S. Mulholland, B. Baptie, J. C. Castellanos, G. Vagenas, J.-O. Gaudron, J. Kronjäger, I. R. Hill, M. Schioppo, I. Barbeito Edreira, K. A. Burrows, C. Clivati, D. Calonico, and A. Curtis, "Optical interferometry–based array of seafloor environmental sensors using a transoceanic submarine cable," Science **376**(6595), 874–879 (2022).
- Q. Zhai, A. Husker, Z. Zhan, E. Biondi, J. Yin, F. Civilini, and L. Costa, "Assessing the feasibility of Distributed Acoustic Sensing (DAS) for moonquake detection," Earth and Planetary Science Letters 635, 118695 (2024).
- S. Coburn, C. B. Alden, R. Wright, K. Cossel, E. Baumann, G.-W. Truong, F. Giorgetta, C. Sweeney, N. R. Newbury, K. Prasad, I. Coddington, and G. B. Rieker, "Regional trace-gas source attribution using a fielddeployed dual frequency comb spectrometer," Optica 5(4), 320 (2018).
- G. Ycas, F. R. Giorgetta, K. C. Cossel, E. M. Waxman, E. Baumann, N. R. Newbury, and I. Coddington, "Mid-infrared dual-comb spectroscopy of volatile organic compounds across long open-air paths," Optica 6(2), 165 (2019).
- T. M. Fortier, M. S. Kirchner, F. Quinlan, J. Taylor, J. C. Bergquist, T. Rosenband, N. Lemke, A. Ludlow, Y. Jiang, C. W. Oates, and S. A. Diddams, "Generation of ultrastable microwaves via optical frequency division," Nature Photon 5(7), 425–429 (2011).
- 11. X. Xie, R. Bouchand, D. Nicolodi, M. Giunta, W. Hänsel, M. Lezius, A. Joshi, S. Datta, C. Alexandre, M. Lours, P.-A. Tremblin, G. Santarelli, R. Holzwarth, and Y. Le Coq, "Photonic microwave signals with zeptosecond-level absolute timing noise," Nature Photon **11**(1), 44–47 (2017).
- C. A. McLemore, N. Jin, M. L. Kelleher, J. P. Hendrie, D. Mason, Y. Luo, D. Lee, P. Rakich, S. A. Diddams, and F. Quinlan, "Miniaturizing Ultrastable Electromagnetic Oscillators: Sub- 10 – 14 Frequency Instability from a Centimeter-Scale Fabry-Perot Cavity," Phys. Rev. Applied 18(5), 054054 (2022).
- M. L. Kelleher, C. A. McLemore, D. Lee, J. Davila-Rodriguez, S. A. Diddams, and F. Quinlan, "Compact, portable, thermal-noise-limited optical cavity with low acceleration sensitivity," Opt. Express **31**(7), 11954 (2023).
- Y. Liu, N. Jin, D. Lee, C. McLemore, T. Nakamura, M. Kelleher, H. Cheng, S. Schima, N. Hoghooghi, S. Diddams, P. Rakich, and F. Quinlan, "Ultrastable vacuum-gap Fabry–Perot cavities operated in air," Optica 11(9), 1205 (2024).
- Y. Liu, D. Lee, T. Nakamura, N. Jin, H. Cheng, M. L. Kelleher, C. A. McLemore, I. Kudelin, W. Groman, S. A. Diddams, P. T. Rakich, and F. Quinlan, "Low-noise microwave generation with an air-gap optical reference cavity," APL Photonics 9(1), 010806 (2024).
- L. Stern, W. Zhang, L. Chang, J. Guo, C. Xiang, M. A. Tran, D. Huang, J. D. Peters, D. Kinghorn, J. E. Bowers, and S. B. Papp, "Ultra-precise opticalfrequency stabilization with heterogeneous III–V/Si lasers," Opt. Lett. 45(18), 5275 (2020).
- J. Alnis, A. Schliesser, C. Y. Wang, J. Hofer, T. J. Kippenberg, and T. W. Hänsch, "Thermal-noise-limited crystalline whispering-gallery-mode resonator for laser stabilization," Phys. Rev. A 84(1), 011804 (2011).
- W. Zhang, F. Baynes, S. A. Diddams, and S. B. Papp, "Microrod Optical Frequency Reference in the Ambient Environment," Phys. Rev. Applied 12(2), 024010 (2019).
- K. Liu, N. Chauhan, J. Wang, A. Isichenko, G. M. Brodnik, P. A. Morton, R. O. Behunin, S. B. Papp, and D. J. Blumenthal, "36 Hz integral linewidth laser based on a photonic integrated 4.0 m coil resonator," Optica 9(7), 770 (2022).
- R. W. P. Drever, J. L. Hall, F. V. Kowalski, J. Hough, G. M. Ford, A. J. Munley, and H. Ward, "Laser phase and frequency stabilization using an optical resonator," Appl. Phys. B **31**(2), 97–105 (1983).
- W. Loh, S. Yegnanarayanan, F. O'Donnell, and P. W. Juodawlkis, "Ultranarrow linewidth Brillouin laser with nanokelvin temperature selfreferencing," Optica 6(2), 152 (2019).

- W. Loh, J. Stuart, D. Reens, C. D. Bruzewicz, D. Braje, J. Chiaverini, P. W. Juodawlkis, J. M. Sage, and R. McConnell, "Operation of an optical atomic clock with a Brillouin laser subsystem," Nature 588(7837), 244– 249 (2020).
- F. Kéfélian, H. Jiang, P. Lemonde, and G. Santarelli, "Ultralowfrequency-noise stabilization of a laser by locking to an optical fiberdelay line," Opt. Lett. 34(7), 914 (2009).
- D. Kwon, C.-G. Jeon, J. Shin, M.-S. Heo, S. E. Park, Y. Song, and J. Kim, "Reference-free, high-resolution measurement method of timing jitter spectra of optical frequency combs," Sci Rep 7(1), 40917 (2017).
- D. Kwon, I. Jeon, W.-K. Lee, M.-S. Heo, and J. Kim, "Generation of multiple ultrastable optical frequency combs from an all-fiber photonic platform," Sci. Adv. 6(13), eaax4457 (2020).
- D. Kwon, D. Jeong, I. Jeon, H. Lee, and J. Kim, "Ultrastable microwave and soliton-pulse generation from fibre-photonic-stabilized microcombs (supplementary)," Nat Commun 13(1), 381 (2022).
- J. Huang, L. Wang, Y. Duan, Y. Huang, M. Ye, L. Liu, and T. Li, "All-fiberbased laser with 200 mHz linewidth," Chin. Opt. Lett. **17**(7), 071407 (2019).
- 28. Y. Huang, D. Hu, M. Ye, Y. Wang, Y. Li, M. Li, Y. Chen, Q. Qu, L. Wang, L. Liu, and T. Li, "All-fiber-based ultrastable laser with long-term frequency stability of 1.1 × 10-14," Chin. Opt. Lett. 21(3), 031404 (2023).
- I. Jeon, C. Ahn, C. Kim, S. Park, W. Jeon, L. Duan, and J. Kim, "Palm-sized, vibration-insensitive, and vacuum-free all-fiber-photonic module for 10–14-level stabilization of CW lasers and frequency combs," APL Photonics 8(12), 120804 (2023).
- L. Duan, "General treatment of the thermal noises in optical fibers," Phys. Rev. A 86(2), 023817 (2012).
- J. Dong, J. Huang, T. Li, and L. Liu, "Observation of fundamental thermal noise in optical fibers down to infrasonic frequencies," Applied Physics Letters 108(2), 021108 (2016).