

# K-SPACE DIFFUSION MODEL BASED MR RECONSTRUCTION METHOD FOR SIMULTANEOUS MULTISLICE IMAGING

Ting Zhao<sup>1,2</sup> Zhuoxu Cui<sup>1</sup> Congcong Liu<sup>1</sup> Xingyang Wu<sup>1</sup> Yihang Zhou<sup>1</sup> Dong Liang<sup>1</sup> Haifeng Wang<sup>1</sup>

<sup>1</sup> Shenzhen Institute of Advanced Technology, Chinese Academy of Sciences, Shenzhen, China

<sup>2</sup> University of Chinese Academy of Sciences, Beijing, China

## ABSTRACT

Simultaneous Multi-Slice(SMS) is a magnetic resonance imaging (MRI) technique which excites several slices concurrently using multiband radiofrequency pulses to reduce scanning time. However, due to its variable data structure and difficulty in acquisition, it is challenging to integrate SMS data as training data into deep learning frameworks. This study proposed a novel k-space diffusion model of SMS reconstruction that does not utilize SMS data for training. Instead, it incorporates Slice GRAPPA during the sampling process to reconstruct SMS data from different acquisition modes. Our results demonstrated that this method outperforms traditional SMS reconstruction methods and can achieve higher acceleration factors without in-plane aliasing.<sup>1</sup>

**Index Terms**— Simultaneous Multi-Slice, Heat Diffusion, MRI, Slice GRAPPA

## 1. INTRODUCTION

Simultaneous Multi-Slice(SMS) is a magnetic resonance imaging (MRI) technique, which utilizes multi-band radiofrequency pulses to simultaneously excite multiple slices, thereby significantly reducing the scanning time of MRI, which is especially important for lengthy acquisitions like diffusion tensor imaging(DTI), volumetric T2-weighted scans and time-resolution applications[1]. Whereas conventional methods have an unavoidable signal-to-noise ratio(SNR) loss, the SNR in SMS scans increases by the square root of the number of slices. Besides, SMS technique reduces the total scanning time by acquiring data from multiple slices within a single TR, but the sequence parameters remain unchanged, having no impact on blurring or distortion.

<sup>1</sup>Ting Zhao and Zhuoxu Cui contributed equally to this work. Some of the work was supported by the National Natural Science Foundation of China (62271474), the National Key Technology Research and Development Program of China (2023YFB3811403, 2023YFC2411103 and 2023YFF0714201), the International Partnership Program of Chinese Academy of Sciences (321GJHZ2023246GC), the Strategic Priority Research Program of the Chinese Academy of Sciences (XDB0930303), the High-level Talent Program in Pearl River Talent Plan of Guangdong Province (2019QN01Y986), and the Guangdong Basic and Applied Basic Research Foundation (2024A1515012138 and 2023B1515120007).

The SMS reconstruction methods include Slice GRAPPA[2] and SENSE-GRAPPA[3]. Based on SENSE GRAPPA, or readout concatenation method (ROC), which creates an extended FOV to separate all the slices, lots of traditional iterative methods and deep learning methods have been proposed like SMS-RAKI[4] and VCC-RAKI[5]. Compared to ROC methods, Slice-GRAPPA based methods has the ability to quantify the slice-leakage artifact “L”-factor but only resolve inter-slice aliasing and require other methods to address intra-slice aliasing issues. Currently, there is a lack of deep learning methods that focus on Slice-GRAPPA because it is challenging to integrate SMS data of different MB and CAIPI forms as training data into deep learning frameworks such as unrolling based method and non-unrolling based method.

Generative deep learning methods such as score based diffusion model do not require paired data to learn the distribution patterns of MR images, therefor avoiding considering SMS data patterns. Based on our previous Slice-Diffusion method[6], we further proposed a novel k-space diffusion framework combining k-space based diffusion model with Slice GRAPPA which combined a forward process trained by single slice MR images and a reverse process constraint with Slice GRAPPA. The final reconstruction outperforms traditional iterative SMS reconstruction methods and is capable of adapting to higher in-plane acceleration factors.

## 2. METHOD


### 2.1. Slice GRAPPA

In Slice-GRAPPA, a separate calibration scan is acquired for each slice and used to estimate a set of slice-specific kernels. The kernels are applied to the SMS data to synthesize an entirely new k-space for each slice. The process of SMS data acquisition can be regarded as:

$$\hat{x}_{00}^{sms} = D\hat{x}^i + n \quad (1)$$

where  $D$  is the encoding matrix,  $n$  is the noise. And Slice GRAPPA kernel  $K$  plays its role in this way:

$$\hat{x}_{aliasing}^i = K\hat{x}_{00}^{sms} \quad (2)$$

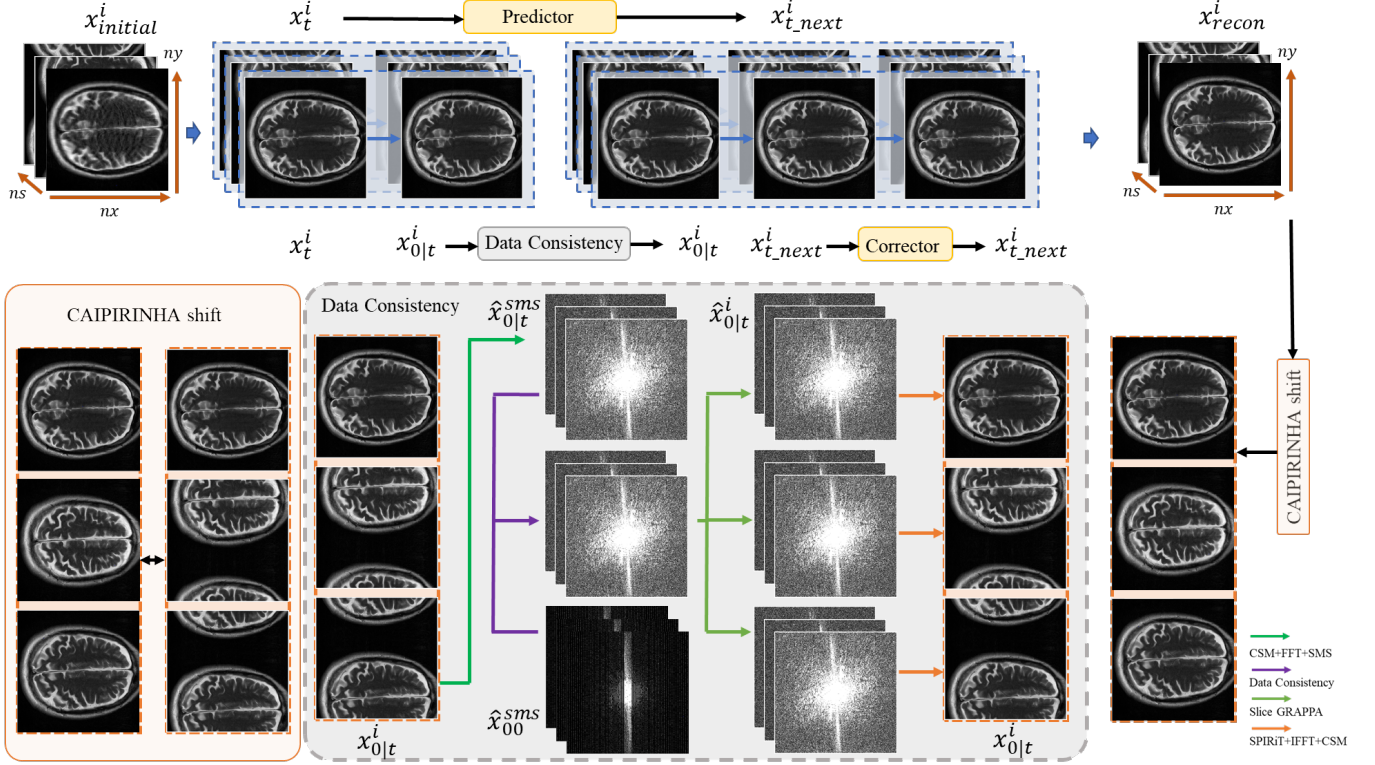

**Fig. 1.** Structure of the SMS Sampling: The SMS sampling begins with the initialized data  $x_{initial}^i$ , and each slice undergoes a predictor and corrector individually. The SMS constraint is included within the data consistency term of the predictor. During Data Consistency term, single slice data  $\hat{x}_{0|t}^i$  are combined to get  $\hat{x}_{0|t}^{sms}$ , and then perform Data Consistency with  $\hat{x}_{00}^{sms}$ , which follows a Slice GRAPPA to obtain each slice again. At the end of reverse diffusion, the CAIPIRINHA shift is applied to get the final reconstruction.

In our proposed method, with the acquired data  $\hat{x}_{00}^{sms}$ , Slice GRAPPA is applied to get initial single-slice data  $\hat{x}_{initial}^i$ . At each step of the sampling process, we reprocess the single-slice data back into the SMS data, conducting data consistency handling during this procedure, and reapply Slice GRAPPA to separate the data.

## 2.2. Heat Diffusion for SMS Reconstruction

In our study, a k-space based diffusion model was used, termed as *heat diffusion*[7]. In Heat Diffusion, the concepts of k-space parallel imaging methods such as GRAPPA and SPIRiT are framed as a process predicting high-frequency missing data based on low-frequency data.

According to Heat Diffusion, the forward SDE is:

$$d\hat{z} = \hat{G}_t \odot \hat{z}(0)dt + \sqrt{\frac{d\sigma^2(t)}{dt}} \overline{SS}^* dw \quad (3)$$

where  $G_t$  is a 2-D Gaussian function,  $\sigma(t)$  is the parameter to control the noise level,  $\overline{S}$  represents  $\mathbb{F}S\mathbb{F}^{-1}$ ,  $S$  denotes coil sensitivity. By introducing noise term, we have modeled k-space attenuation as SDE. In contrast to the heat equation, the reverse SDE for equation (3) reads:

$$d\hat{z} = [\hat{G}_t \odot \hat{z}(0) - \frac{d\sigma^2(t)}{dt} \overline{SS}^* \nabla_{\hat{z}} \log p_t(\hat{z})]dt + \sqrt{\frac{d\sigma^2(t)}{dt}} \overline{SS}^* d\bar{w} \quad (4)$$

Reverse SDE involves an unknown function  $\nabla_{\hat{z}} \log p_t(\hat{z})$ , the score-matching loss function is reduced to:

$$\theta^* = \underset{\theta}{\operatorname{argmin}} \mathbb{E}_t \{ \lambda(t) \mathbb{E}_{\hat{z}(t)} \mathbb{E}_{\hat{z}(t)|\hat{z}(0)} [ \| \overline{S}^* (\hat{G}(t) \odot (h_{\theta}(\hat{z}(t), t) - \hat{z}(0))) \|_2^2 ] \} \quad (5)$$

where  $h_{\theta}(\hat{z}(t), t)$  means the network. Based on the modeling of forward and reverse attenuated k-space diffusion, the following equation:

$$\hat{z}_i = \hat{z}_{i+1} - (\hat{G}_{i+1} - \hat{G}_i) \odot \hat{z}_0 + \sqrt{\sigma_{i+1}^2 - \sigma_i^2} \overline{SS}^* n + (\sigma_{i+1}^2 - \sigma_i^2) \overline{SS}^* \nabla_{\hat{z}_{i+1}} \log p_{i+1}(\hat{z}_{i+1}) \quad (6)$$

enables the reconstruction of missing high-frequency k-space data using low-frequency ACS data.

### 2.3. SMS Sampling

Due to the distinct multiband (MB) acceleration and complex additional parameters in SMS imaging, such as different CAIPIRINHA shift type, training holistically within the diffusion process is exceedingly intricate. Therefore, single-slice images are utilized for training, enabling the k-space-based diffusion model to learn the overall distribution of MRI images in k-space. During the sampling process, the physical model of SMS is integrated to reconstruct SMS data. The specific reconstruction workflow is depicted in Figure 1:

Before the sampling steps, data initialization is needed. Firstly applying Slice GRAPPA to SMS data to obtain single-slice data with in-plane aliasing. Then, SPIRiT was applied for each slice. Following this initialization, these data were prepared to undergo the reverse diffusion process.

## 3. EXPERIMENT

### 3.1. Dataset

FastMRI Dataset was used to train the Heat Diffusion Model. For sampling test, we simulated SMS data using fastMRI T2 brain dataset and cropped the image to 320 x 320. We set MB=3 with different in-plane acceleration factors. To ensure minimal inter-slice leakage, a 2/3 field-of-view (FOV) CAIPIRINHA shift was applied to the three images, and the central region of k-space was extracted as 32 ACS lines. The corresponding Slice GRAPPA kernel was obtained using the ACS data, along with the SPIRiT kernel for each slice and the coil sensitivity maps.

### 3.2. Performance Evaluation

For quantitative evaluation, the peak signal-to-noise ratio (PSNR), normalized mean square error (NMSE) value and structural similarity (SSIM) index were adopted on the image domain.

## 4. RESULTS AND DISCUSSION

### 4.1. Compared to traditional SMS methods

The methodology proposed in this study was compared with traditional Slice-GRAPPA+SNESE and SMS-COOKIE[8]. The uniform undersampling mask was used, with in-plane undersampling factors of 3x and 4x. Results of 4x are shown in Fig.2. Under the condition of 4x, the Slice GRAPPA+SENSE and SMS-COOKIE introduced obvious in-plane aliasing, whereas our proposed method demonstrated better reconstruction results, without in-plane aliasing better high-frequency details. Detailed performance is presented in Table 1.

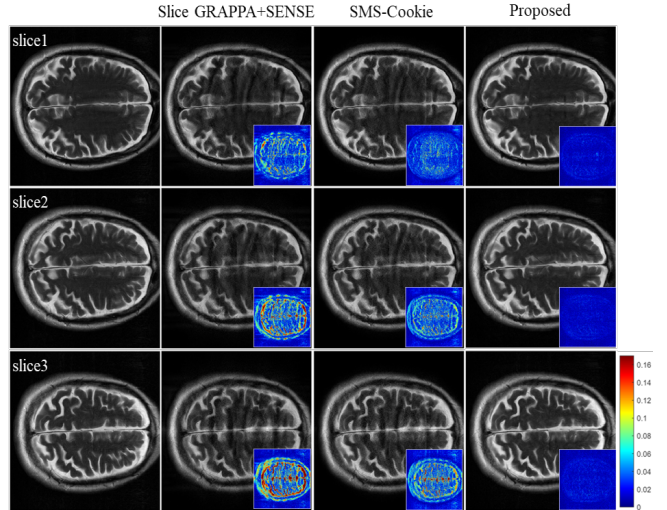


Fig. 2. Reconstruction Results of Different Method in 4X

	NMSE	PSNR	SSIM
Slice GRAPPA+SENSE(3x)	0.0291	30.7509	0.8069
SMS-COOKIE(3x)	0.0261	31.6853	0.7446
Proposed(3x)	<b>0.0125</b>	<b>38.0801</b>	<b>0.9463</b>
Slice GRAPPA+SENSE(4x)	0.0614	24.4251	0.7317
SMS-COOKIE(4x)	0.0445	27.1895	0.6839
Proposed(4x)	<b>0.0143</b>	<b>36.9111</b>	<b>0.9356</b>

Table 1. Quantitative Comparison for Different Method

### 4.2. Different in plane acceleration factors

Traditional SMS reconstruction methods are typically limited in in-plane acceleration factors, with noticeable aliasing artifacts emerging at high acceleration, as shown in Fig.2. However, due to the superior reconstruction performance of Heat Diffusion, greater breakthroughs can be achieved in in-plane reconstruction factors. The following figures present the reconstruction results of the model proposed in this study under various in-plane acceleration factors. As illustrated, the method proposed does not exhibit undersampling artifacts even at 8x. Nevertheless, due to the loss of high-frequency information at higher acceleration factors, some image details gradually become blurred or even disappear as the acceleration factor increases.

### 4.3. Discussion


We also tried the SMS test data processed by slice GRAPPA using the end-to-end method H-DSLRL[9] and the unrolling method MoDL[10], but it is challenging for the frameworks of these methods to be compatible with SMS reconstruction based on slice GRAPPA. Therefore, the proposed SMS reconstruction method based on generative diffusion models has

	NMSE	PSNR	SSIM
acc3	0.0125	38.0801	0.9463
acc4	0.0143	36.9111	0.9356
acc5	0.0163	35.7503	0.9285
acc6	0.0211	33.7523	0.9182
acc7	0.0212	33.5225	0.9123
acc8	0.0305	30.4993	0.8954

**Table 2.** Quantitative Comparison for Different Acc

significant advantages.

Besides, our current method still has some limitations. At high in-plane acceleration factors, although PSNR and SSIM still maintain relatively high values, the NMSE values indicate that further optimization is needed in terms of high-frequency details. Subsequently, we will add additional constraints to address this issue and compare our method with more methods in multiple dimensions.

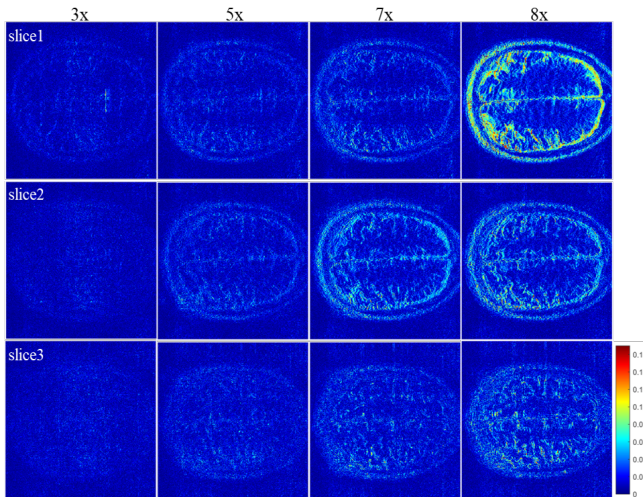

**Fig. 3.** Error Map of Different In-plane acc

## 5. CONCLUSION

This study proposed a SMS reconstruction method based on Heat Diffusion and slice GRAPPA. Our proposed method does not require SMS data for training, thereby avoiding issues associated with the variability and difficulty in obtaining SMS dataset. Moreover, due to the superior reconstruction performance of diffusion model, our proposed reconstruction method is less likely to exhibit undersampling aliasing artifacts even when using higher in-plane acceleration factors. Compared to traditional SMS reconstruction methods, our method demonstrates superior reconstruction performance.

## 6. REFERENCES

- [1] Markus Barth et al., “Simultaneous multislice (sms) imaging techniques,” *Magnetic resonance in medicine*, vol. 75, no. 1, pp. 63–81, 2016.
- [2] Kawin Setsompop et al., “Blipped-controlled aliasing in parallel imaging for simultaneous multislice echo planar imaging with reduced g-factor penalty,” *Magnetic resonance in medicine*, vol. 67, no. 5, pp. 1210–1224, 2012.
- [3] Martin Blaimer et al., “Accelerated volumetric mri with a sense/grappa combination,” *Journal of Magnetic Resonance Imaging: An Official Journal of the International Society for Magnetic Resonance in Medicine*, vol. 24, no. 2, pp. 444–450, 2006.
- [4] Chi Zhang et al., “Accelerated simultaneous multi-slice mri using subject-specific convolutional neural networks,” in *2018 52nd Asilomar Conference on Signals, Systems, and Computers*. IEEE, 2018, pp. 1636–1640.
- [5] Wanting Wang et al., “Reconstruction of simultaneous multi-slice mri data by combining virtual conjugate coil technology and convolutional neural network,” *Chinese Journal of Magnetic Resonance*, vol. 37, no. 4, pp. 407–421, 2020.
- [6] Ting Zhao et al., “Mr optimized reconstruction of simultaneous multi-slice imaging using diffusion model,” *2024 Proc. of the International Society for Magnetic Resonance in Medicine (ISMRM)*, 2024.
- [7] Zhuo-Xu Cui et al., “Physics-informed deepmri: Bridging the gap from heat diffusion to k-space interpolation,” *arXiv preprint arXiv:2308.15918*, 2023.
- [8] Ömer Burak Demirel et al., “Improved simultaneous multi-slice imaging with composition of k-space interpolations (sms-cookie) for myocardial t1 mapping,” *PloS one*, vol. 18, no. 7, pp. e0283972, 2023.
- [9] Aniket Pramanik et al., “Deep generalization of structured low-rank algorithms (deep-slr),” *IEEE transactions on medical imaging*, vol. 39, no. 12, pp. 4186–4197, 2020.
- [10] Hemant K Aggarwal et al., “Modl: Model-based deep learning architecture for inverse problems,” *IEEE transactions on medical imaging*, vol. 38, no. 2, pp. 394–405, 2018.