

Optical detection of cancer stages via partial wave spectroscopy (PWS) using tissue microarrays (TMA) samples

Prakash Adhikari and Prabhakar Pradhan*

Department of Physics and Astronomy, Mississippi State University, Mississippi State, MS 39762, USA

**Corresponding author: pp838@msstate.edu*

Abstract

The progression of cancer is associated with different genetic and epigenetic events which result in nano to microscale structural alterations in cells/tissue. However, these structural alterations in the early stage of the disease remain undetectable by conventional microscopy due to the diffraction-limited resolution of $\sim 200\text{nm}$. With cancer being an epidemic worldwide, early and accurate detection methods are always in demand. In this sense, we developed a finer focusing mesoscopic physics-based partial wave spectroscopy (PWS) imaging and quantification technique, which can probe the precise scattering volume in cells/tissue to detect such structural alterations. Therefore, we employ the highly sensitive PWS technique to quantify the nanoscale refractive index fluctuations using commercially available paraffin embedded tissue microarrays (TMA) samples with the goal of the standardized early and accurate detection of stages of different cancers. Recently the use of scientific TMA samples has gained research interest in diagnosing different diseases and drug-effect in treatment since they are commercially easily accessible. In this work, deadly cancer such as pancreatic, prostate, breast, and colon cancer TMAs containing multiple cores of different stages for each cancer are analyzed using the PWS technique and the degree of disorder strength L_d was quantified. The finer focusing PWS results show that an increase in the disorder strength with the increase in the stage of each cancer. This quantitative analysis of different cancer stages using commercially available TMA samples could enhance and standardize early, accurate cancer diagnosis modalities.

Keywords: *Spectroscopy, Optical detection, Disorder strength, Cancer, Tissue microarrays (TMA)*

Introduction:

The optical detection of structural changes in biopsy samples due to progressive cancer has achieved tremendous success in detecting the stages of cancer when developed into a tumor (1). The standard pathological method of detection of cancer stages includes microscopic examination of the morphological changes using stained biopsy samples. However, due to the diffraction limited resolution of the conventional microscopy, the structural alterations in healthy tissue before the development of a tumor or early stages are still a mystery. These structural alterations of healthy cells/tissue are due to the rearranging of macromolecules such as DNA, RNA, lipids, etc.

whose size ranges 100-200 nm. It is recognized that genetic and epigenetic alterations occur not only at the neoplastic focus but more diffusely in field cancerization. The abnormalities are present in the tissue surrounding the cancerous region or transformed cell primary tumor due to field cancerization (2,3), which are initially at the nanoscale level before tumor formation and migration. This effect is observed in almost every type of cancer that is diagnosed in the later stages with almost no hope of survival due to metastasis of cancer cells. Therefore, a highly sensitive optical method to detect such structural abnormalities before the development of a tumor for all cancer is paramount for decreasing lethality (4). With the progress of time, several microscopic imaging techniques were employed, and regardless of their drawbacks, significant success was achieved (5). Unfortunately, most of these methods are still not sensitive enough to probe the nanoscale structural changes. In light of this scenario, the versatile approach of using recently developed partial wave spectroscopy (PWS) to probe the refractive index fluctuations in commercially available tissue microarray (TMA) samples could standardize the cancer diagnostic modalities. The recently developed finer focusing PWS technique, a furthered technique, is sensitive enough to probe nanoscale refractive index fluctuations in paraffin embedded TMA samples. The PWS combines interdisciplinary approaches of mesoscopic physics and optical imaging techniques to quantify the degree of disorder strength (L_d) based on refractive index fluctuations within the cells/tissue (6–9). The backscattered signal at any point within a weakly disordered medium contains the spectral fluctuations which are proportional to the local density of macromolecules or refractive index fluctuations, in fact, independent of chemical composition. Thus, once the refractive index fluctuations of the medium are known, the spatial variations of macromolecular density can be measured using the disorder strength (L_d) as $L_d = \langle dn^2 \rangle l_c$, where $\langle dn^2 \rangle$ is the *rms* and l_c is the correlation length of the refractive index fluctuations (6,7). This potential biomarker, the L_d parameter has shown tremendous success in distinguishing stages of cancer, drug-effect in cancer treatment, and to quantify any other type of abnormalities in the brain (6,8,10–12). In addition to this, structural alterations in biological cells/tissue due to cancer or in any other abnormalities are quantified using mesoscopic physics-based molecular specific light localization technique in terms of the degree of disorder strength (13–16).

With the availability of such a powerful approach to quantify the nanoscale structural alterations in cancerous tissue, the next challenge was in the use of an almost identical tissue sample that allows high-throughput analysis to standardize diagnostic techniques. For this, the

recently developed commercially available TMAs have been used which significantly facilitate and accelerates tissue analyses using a highly sensitive PWS technique. The TMA is a scientific form of condensed histopathology where the tissue is kept in a single glass slide to provide a miniature multiplex platform for analysis (17). Multiple cores of paraffin embedded tissue in a TMA allow high-throughput assessment of macromolecules in PWS analysis that standardize the diagnostic technique reducing the variability seen on the assay of individual samples. This uniformity of assay has reduced the drawbacks in specimen handling and their impact on data acquisition (18). Besides these facts, TMA samples are easily accessible to perform any scientific experiments which require more than one similar sample. Also, we believe the use of the PWS technique in the TMA sample could be a new direction to explore to study the drug-effect on cancer or any other abnormalities that are in demand.

In this paper, four different deadly cancer TMAs: *pancreatic*, *breast*, *colon*, and *prostate* were studied and generalize the efficacy of developed finer focusing PWS to detect the cancer stages. Cancer is a common disease and with no surprise, these four different cancers are the major cause of death in the U.S. Because of lethality, prevalence, and almost no prominent physical change or symptoms until the later stages. We focus on studying the nanoscale structural changes in these cancerous tissues by quantifying the degree of disorder (L_d) as a potential biomarker. In this sense, we explored the potential possibilities of the PWS technique in TMAs for the early stage of cancer detection.

Methods:

1.1 Experimental Setup:

The engineered finer focusing PWS system used to probe the precise scattering volume developed in the Bionanophonics laboratory is as shown in fig. 1. The details of the PWS experimental setup is presented elsewhere (8,10,12,19). However, in brief, the developed PWS system consists of a low coherence broadband stable white light source Xenon lamp (150W) which is reflected toward the 4f combination of lenses by a mirror and gets collimated. Collimated beams are reflected towards the 40X objectives and focus on the sample with the help of a highly sensitive XYZ motorized scanning stage (XY-axis 40nm and Z-axis 100nm). Then, the backscattered signal from the sample is directed towards the CCD camera through the liquid crystal tunable filter (LCTF)

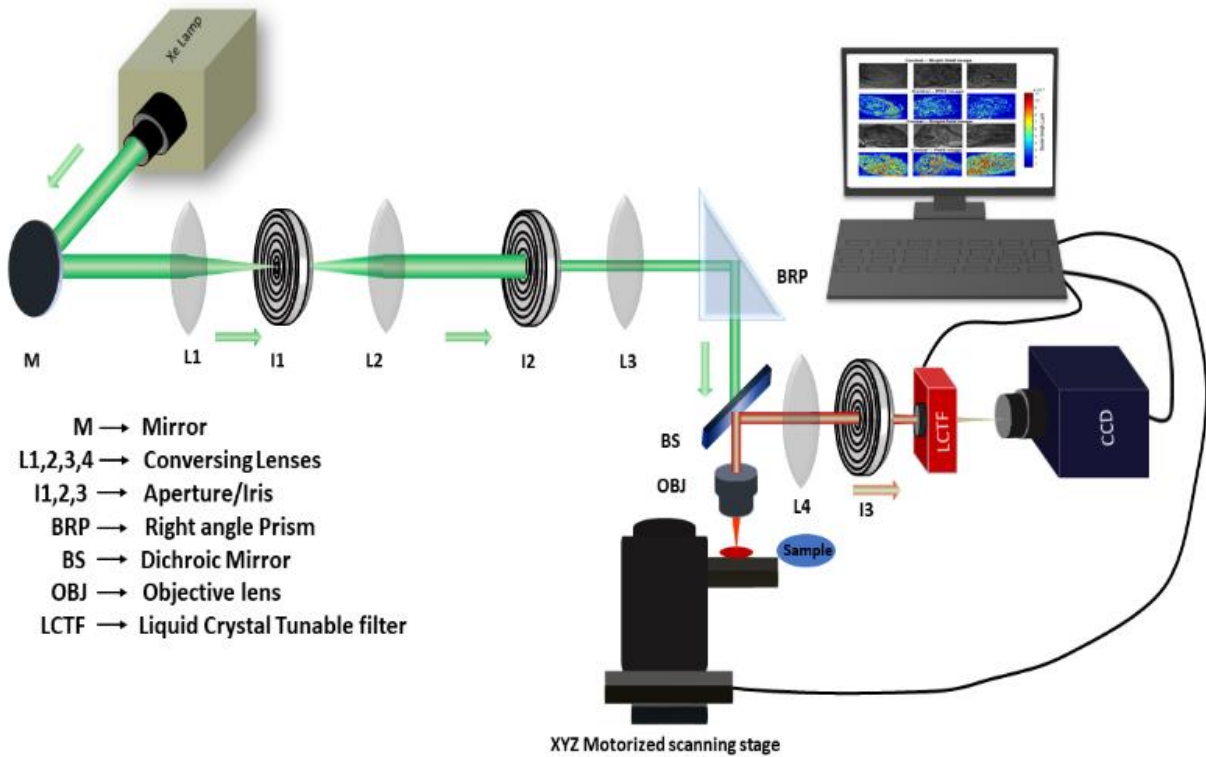


Fig. 1. The schematic layout of the finer focusing partial wave spectroscopy (PWS) system. The collimated beam (green color) from broadband stable white light source is focus into the sample and the reflected signals (red color) from the sample are collected by the CCD.

with the help of a dichroic mirror. The LCTF has a resolution of 1nm in the visible range of light (420-730nm). Here, LCTF is coupled with a CCD camera in a way that for every wavelength in the visible range, images are recorded in the CCD camera for the PWS analysis.

1.2 Calculation of the disorder strength (L_d):

In the PWS technique, the backscattered spectrum of a weakly disorder medium is recorded in the visible range of light to quantify the degree of disorder strength (L_d) based on the refractive index fluctuations ($dn(z)$) within the cells/tissue. It is shown that at each pixel position (x,y) within the cell, the refractive index (n) is proportional to the local mass density and practically independent of chemical composition at that point. Therefore, the spatial variation of macromolecular mass density at every pixel position can be expressed in terms of refractive index fluctuations, assuming that these random fluctuations are within a correlation length (l_c). The recorded backscattered

spectrum $R(x, y; \lambda)$, is the interference between the intercellular volume scattering and reflection from the surface of the sample. That means the measured spectra from each pixel of an image is a 1D weakly disordered medium which acts as a subset of the scattered waves.

In 1D weakly disorder medium, the probability density distribution of reflectance fluctuations R , follows a log-normal distribution for all the sample length scale L within the scattering medium. As mentioned, PWS collects the backscattered signals propagating along the 1D trajectories since in a quasi-1D approximation the sample is virtually divided into many parallel channels within the diffraction-limited transverse size. Then, by applying mesoscopic light transport theory and making use of refractive index fluctuations, the degree of disorder strength is calculated. In particular, the *rms* value of the reflection intensity $\langle R(k) \rangle_{rms}$ and the spectral auto-correlation of the reflection intensity $C(\Delta k)$ for a given pixel at position (x,y) , are combined to define the degree of disorder strength as (6,7,20):

$$L_d = \frac{B n_0^2 \langle R \rangle_{rms}}{2k^2} \frac{(\Delta k)^2}{-\ln(C(\Delta k))} \Big|_{\Delta k \rightarrow 0}$$

Where B is the normalization constant, n_0 is the average refractive index of the weakly disordered medium, k is the wavenumber ($k = 2\pi/\lambda$), and $(\Delta k)^2/\ln(C(\Delta k))$ is obtained by performing a linear fit of $\ln(C(\Delta k))$ vs $(\Delta k)^2$.

For the Gaussian color noise of the refractive index at position r and r' , $\langle dn(r)dn'(r') \rangle = dn^2 \exp(-|r-r'|/l_c)$, then L_d can be expressed as $L_d = \langle dn^2 \rangle l_c$ (7,9). Therefore, the average and standard deviation (*std*) of the disorder strength quantifies the variability of the local density of intracellular material within the samples.

1.3 Tissue Microarrays (TMA) samples:

TMA is a rapidly growing commercially available research mechanism that consists of numerous different cases of 5 μ m thick tissue cores in diameter 1.5mm placed on the same glass slide for simultaneous analysis. These paraffin embedded TMA samples allow the high-throughput analysis of tissue samples since different cases of samples have exact experimental conditions and batches of reagents. TMAs are therefore scientific, cost-efficient, and offer an unprecedented degree of standardization for the conduction of an experiment such as optical imaging (21), especially at the research and development level, at the beginning.

Here, using the PWS, we quantify the structural properties of paraffin embedded TMAs from US Biomax of the pancreas (T142b), breast (BR248a), colon (T054c), and prostate (T191a) due to progressive carcinogenesis. Each TMA consists of different cores of normal, stage I, stage II, and stage III cancer tissue samples. Different cores of each TMAs are from individual patients of varying ages and sex. However, for each stage of each cancer, at least two different cores of the same age and sex were analyzed to calculate the degree of structural disorder.

Results and Discussion:

To develop a standardized diagnostic test for early and effective detection of stages of varying types of the deadliest cancers, the structural abnormalities were quantified using a finer focusing PWS technique of TMAs. Here, the degree of disorder strength (L_d) for different stages of pancreatic, breast, colon, and prostate cancer TMAs were computed and compared. The results show that structural alterations increase with the progression of cancer stages in each type of progressive cancer. Since the disorder strength (L_d) is the product of the variance and spatial correlation length of the refractive index fluctuations, $L_d = \langle dn^2 \rangle l_c$, these results indicate that the progression of cancer increases more mass accumulations in the tissue results in increasing the refractive index fluctuations increasing the L_d . In addition to the earlier findings, this work explores the application of the developed, highly sensitive PWS technique to detect the nanoscale fluctuations in paraffin embedded TMA tissue samples of four different deadly cancers.

For each type of cancer TMA samples: *pancreatic*, *breast*, *colon*, and *prostate* tissue PWS spectroscopic images were recorded in the visible range (450-700nm) of light from three different cores of the same type. From each core, at least 5 different realizations were made for the PWS analysis. Using this powerful spectroscopic technique, the pixel-wise refractive index fluctuations of tissue were computed and first represented in the 2D L_d map/image. Then, the ensemble average and standard deviation (*std*) of the disorder strength (L_d) were computed and presented in a bar graph for all cancerous TMAs studied.

Pancreatic cancer:

Pancreatic cancer is a lethal condition worldwide due to poor outcomes and a rising incidence rate. It is further predicted as one of the leading causes of cancer deaths in the US and often presents at an advanced stage which contributes to a poor five-year survival rate (22). Because of its physical orientation and lack of early symptoms, a better understanding of the symptoms associated with

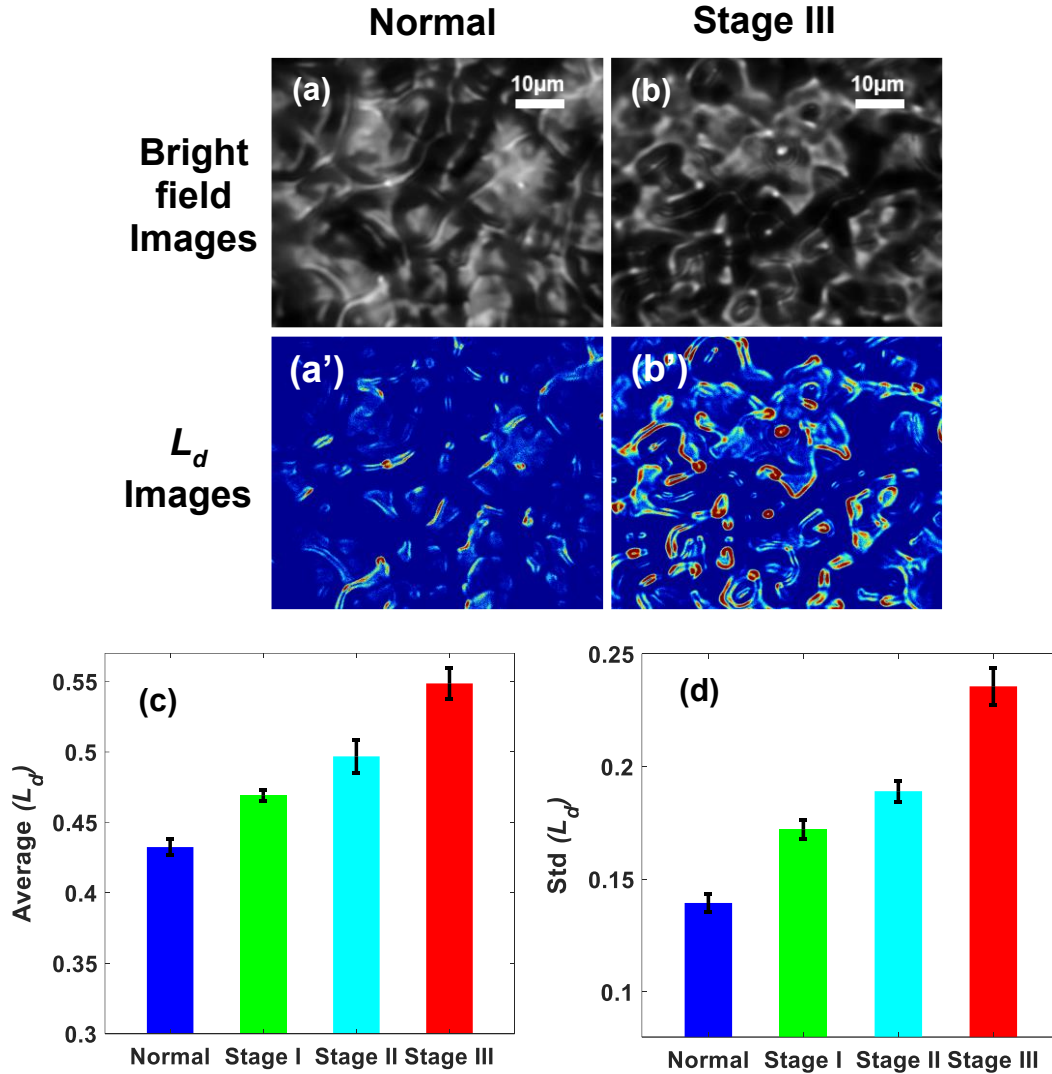


Fig. 2. Pancreatic cancer: (a) and (b) are the representative bright field images of normal and stage III pancreatic cancer TMA tissue while (a') and (b') are their corresponding L_d images. (c) and (d) are the bar graph representation of the average and *std* of disorder strength (L_d) for normal and different stages of pancreatic cancer TMA. The PWS analysis of TMA tissues shows that both the average and *std* of L_d value increases from the normal to higher stages of pancreatic cancer. In reference to the normal, the *std* of L_d value of cancer stage I is 23%, stage II is 36%, stage III is 69% higher (Students ttest P -value < 0.001 , $n=15$).

pancreatic cancer and its risk factor is essential to both health professionals and individuals. Therefore, we focus our research with added finer focusing on the existing PWS technique for the early diagnosis and to understand the structural properties of pancreatic tissue with progressive carcinogenesis using TMA tissue. The results show that mass density or refractive index fluctuations increase with the increase in pancreatic cancer stages. Fig 2. (a)-(b) and (a')-(b') are the representative bright-field and their corresponding L_d images of normal and stage III

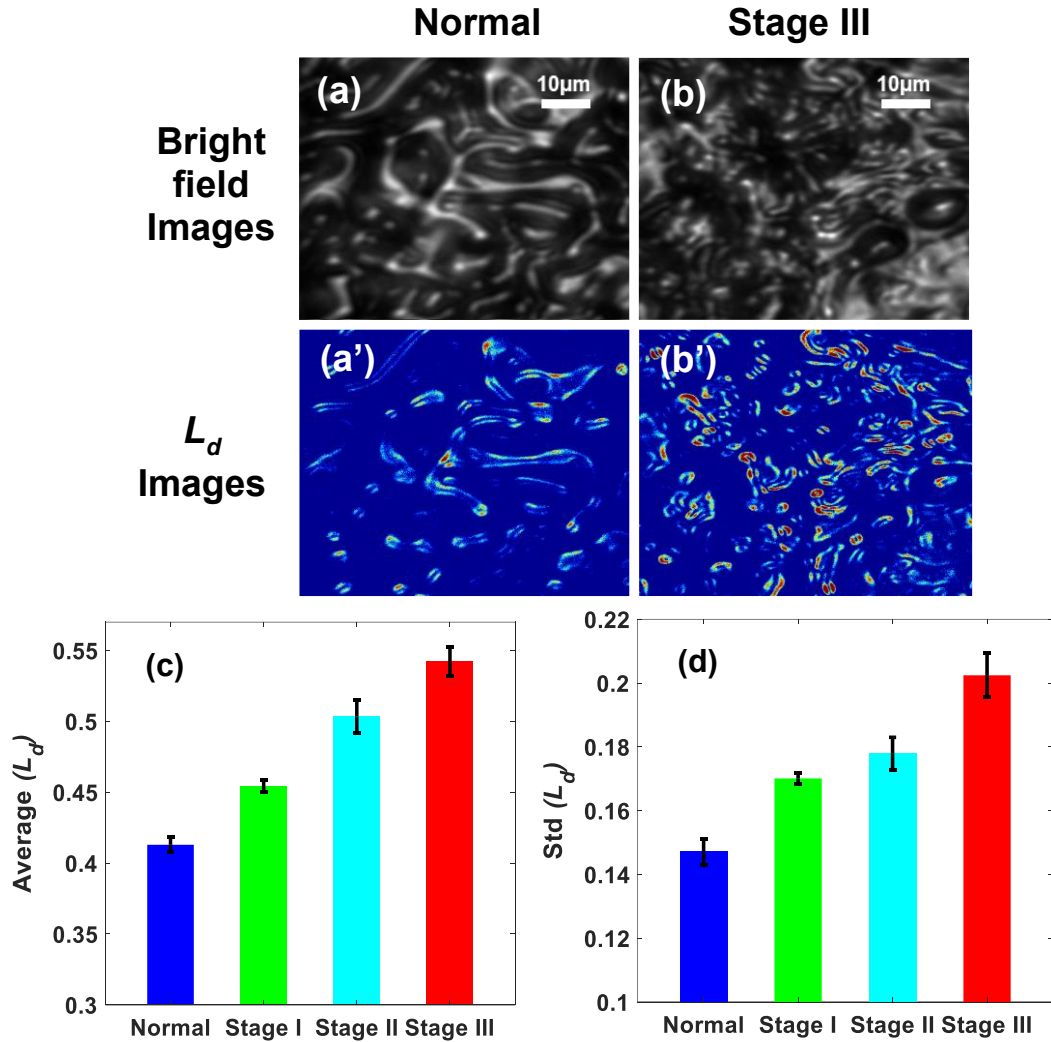


Fig. 3. Breast cancer: (a) and (b) are the bright field images while (a') and (b') are the L_d images of the normal and stage III breast cancer of TMA tissue, respectively. (c) and (d) are the bar graphs of average and *std* of disorder strength (L_d) for the normal and different stages of breast cancer TMA samples. The PWS result using TMA tissue shows that both the average and *std* of L_d value increases from normal to higher stages of cancer tissue. In reference to the normal, the *std* of L_d value of cancer stage I is 16%, stage II is 21%, stage III is 38% higher (Student ttest P -value < 0.001, n=15).

pancreatic cancer tissue. The L_d map, which is a 2D image average along the z-axis represents the refractive index fluctuations at that point. The L_d map shows stage III pancreatic cancer sample has more red spots which indicate higher refractive index fluctuations in the color map. Further, the average and *std* of the degree of disorder strength were calculated and represented in the bar graph, Fig. 2. (c)-(d). Both the average and *std* of L_d value increase from normal, to stage I, stage

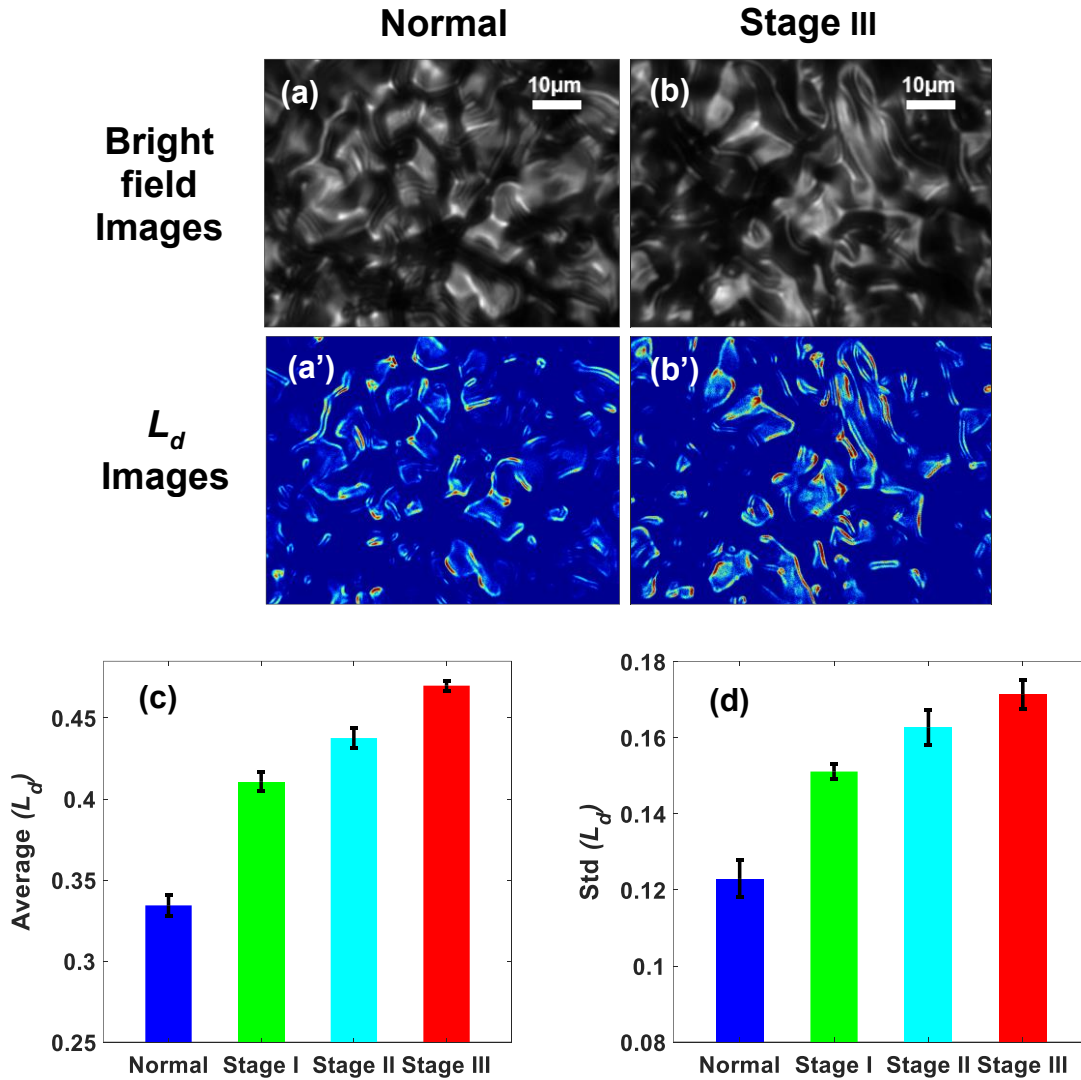


Fig. 4. Colon cancer: (a) and (b) are the bright field images of the normal and stage III colon cancer TMA tissue and (a') and (b') are their respective L_d Images. (c) and (d) bar graphs of the average and *std* of disorder strength (L_d) for the normal and different stages of colon cancer TMA. The PWS result of TMA tissue shows that the average and *std* of L_d value increases from normal to higher stages of colon cancer. In reference to the normal, the *std* of L_d value of cancer stage I is 23%, stage II is 32%, stage III is 40% higher (Student ttest P -value < 0.001 , $n=15$).

II, stage III with a significant difference (Student t-test p -value < 0.001). This result, therefore, suggests that the developed finer focusing PWS technique is sensitive enough to detect nanoscale refractive index fluctuation and to distinguish the different stages of cancer in paraffin embedded pancreatic TMA samples.

Breast cancer:

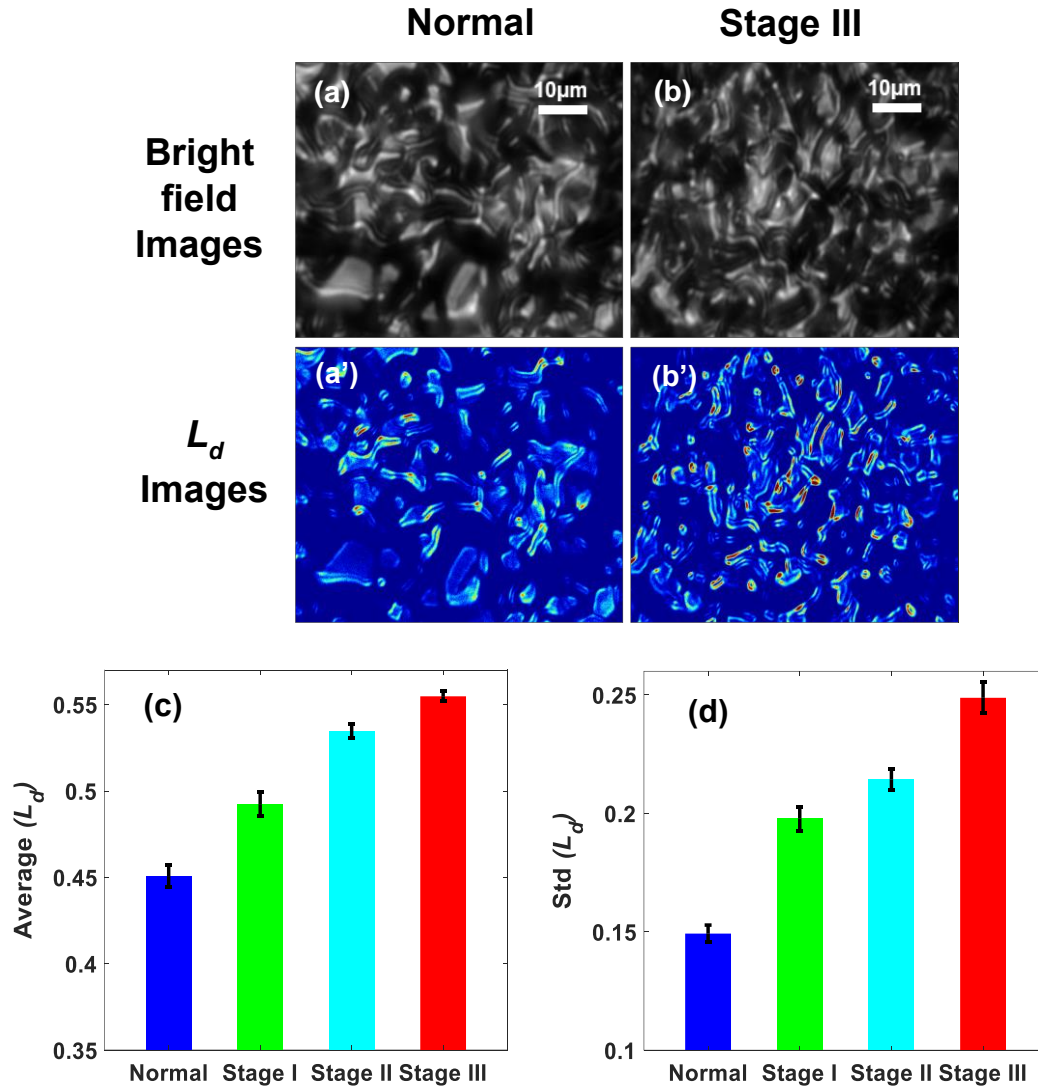


Fig. 5. Prostate cancer: (a) and (b) are the representative bright field images of the normal and stage III prostate cancer TMA tissue while (a') and (b') are their corresponding L_d images. (c) and (d) are bar the graphs of the average and *std* of disorder strength (L_d) for the normal and different stages of prostate cancer TMA. The PWS analysis of TMA tissue show both the average and *std* L_d value increases from the normal to higher stages of cancer tissue. In reference to the normal, the *std* L_d value of cancer stage I is 32%, stage II is 46%, and stage III is 65% higher (Student ttest P -value < 0.001 , $n=15$).

Breast cancer is the most common cancer in women and a challenging cause of cancer death in the world. This metastatic cancer is transferable to different organs such as the bones, lungs, liver, and brain with almost incurability. Early diagnosis of breast cancer is only the best method of prevention. Although the five-year relative survival rate of an early detected breast cancer patient is more than 80% nowadays, oncologists and scientists are still struggling to develop a technique

that can identify early symptoms and distinguish the nanoscale structural changes in breast cancer cells/tissue (23). In the existing scenario, the finer focusing PWS technique was applied to characterize the structural properties of breast cancer TMA tissue samples at the nanoscale level due to progressive carcinogenesis. The result shows that the structural disorder (L_d) increases from the normal to stage III significantly as shown in fig. 3. The representative L_d images fig. 3. (a')-(b') for normal and stage III cancer were presented which show that the refractive index or mass density fluctuations are higher in stage III breast cancer. Also, the average and *std* of L_d value increase significantly from stage I, stage II, to stage III about the normal with Student t-test *p-value* < 0.001 as represented in fig. 3. (c)-(d). This increase in the degree of disordered strength due to progressive carcinogenesis indicates that the refractive index fluctuations increase with the stages of cancer which was successfully detected by finer focusing PWS using TMA tissue samples.

Colon cancer:

Colorectal cancer is the predominant cancer accounting for approximately 10% of all cancer mortality in the world. Population aging, improper dietary habits, smoking, low physical activity, and obesity are the main reasons for annually increasing metastatic colorectal cancer cases (24,25). Until modern times, laparoscopy surgery has played a vital role in controlling or treatment for primary and metastatic colorectal cancer. Despite advances in surgical and medical therapies, the long survival rate of colorectal patients has changed very little in recent times. This demands standardization in screening or imaging techniques to detect the early stages of colon cancer. Therefore, to understand the structural changes in cells/tissue at the nanoscale level due to progressive colon cancer we apply the PWS technique to distinguish different stages of cancer in colon TMA tissue samples. The averages and *std* of the degree of disorder strength (L_d) increase from the normal to stage III with a significant difference (Student ttest *p-value* < 0.005). As cancer increases, mass density accumulation increases which in turn increases the refractive index fluctuations resulting in increased L_d value for higher cancer stages. In addition to this, the L_d images were also constructed to visualize how the refractive index fluctuations increase with the increase in cancer stages in colon TMA samples and shown in fig 4. (a')-(b'). The bar graphs show that the average and *std* of L_d value increases in stage I, stage II, and stage III cancer compare to normal and this result is presented in Fig. 4 (c)-(d).

Prostate cancer:

Prostate cancer is common cancer among men, especially elderly ones and 1 in 9 men will have prostate cancer during their lifespan. Ceasing to smoke, proper exercise, and weight control are good health practices that may reduce the risk of developing prostate cancer. Although remarkable progress has been achieved on characterizing risk factors and identifying therapeutic treatment options. Screening for and diagnosing the early stages of prostate cancer is still one of the most challenging issues across the globe in medicine (26,27). At this point, the study of structural properties of prostate cancer tissue at the nanoscale level using a precise volume scattering technique, PWS of TMA tissue could help to characterize the structural change in their stage. The results obtained using the PWS technique to study the commercially available prostate TMA samples is presented in fig 5. The representative L_d images i.e. fig. 5(a')-(b') shows that stage III Prostate cancer has more red spots because it has a higher mass density or refractive index fluctuations than normal. To quantify the structural abnormalities, the average and *std* of the degree of disorder strength (L_d) were computed and represented in the bar graph, as shown in fig. 5. (c)-(d). As can be seen from the figure, both the average and *std* of L_d value increase in stage I, stage II, and stage III compared to normal. This increase in the L_d is due to the increase in refractive index fluctuations with the increase in the stages of prostate cancer.

Conclusions:

In summary, as an alternative method in cancer research of applying the mesoscopic physics-based PWS technique using commercially available TMA samples has been reported. This technique makes the use of the recently developed finer focusing PWS technique which can control the scattering from precise sample volume to detect the nanoscale structural changes in paraffin embedded tissue and distinguishes the stages of different cancer. To validate the purpose method, the degree of disorder strength (L_d) of different tissue with the progression of cancer stages of commercially available different TMAs are quantified. The PWS results obtained for some of the deadliest cancer TMAs: *pancreatic, breast, colon, and prostate* show that the average and *std* disorder strength (L_d) increases significantly as cancer progresses through the different stages. However, the more prominent changes were found in the *std* of the degree of L_d value for all case

studies. The results provided by the purposed method were in accordance with the earlier studies (6,10) and therefore, the L_d parameter acts as a potential biomarker to distinguish and standardize the cancer stages which seems almost impractical. In addition to this, the use of the PWS technique and commercially available TMAs could provide an easy and scientific way to access the samples and study the drug-effect in cancer treatment, in a larger scale. In particular, this finding invites the research communities to work with a common goal to standardize early, accurate detection, progress of cancer stages, and effect of drugs for different types of deadly cancer cases. Further validation in distinguishing the stages of cancer of TMA tissue can be performed using other quantitative approaches such as fractal, Inverse participation ratio (IPR), etc. (14,28,29). Lastly, the flexibility provided using the spectroscopic technique such as PWS in commercially available TMA samples to distinguish the early stage of cancer and opens a broad way to explore and generalize the structural changes in progressive cancer for effective diagnosis and drug treatment in the future.

Acknowledgements:

This work is partly supported by the Mississippi State University.

References:

1. Huang X, El-Sayed MA. Gold nanoparticles: Optical properties and implementations in cancer diagnosis and photothermal therapy. *Journal of Advanced Research*. 2010 Jan 1;1(1):13–28.
2. Damania D, Roy HK, Subramanian H, Weinberg DS, Rex DK, Goldberg MJ, et al. Nanocytology of Rectal Colonocytes to Assess Risk of Colon Cancer Based on Field Cancerization. *Cancer Res*. 2012 Jun 1;72(11):2720–7.
3. Slaughter DP, Southwick HW, Smejkal W. “Field cancerization” in oral stratified squamous epithelium. Clinical implications of multicentric origin. *Cancer*. 1953;6(5):963–8.

4. O'Shaughnessy JA, Kelloff GJ, Gordon GB, Dannenberg AJ, Hong WK, Fabian CJ, et al. Treatment and Prevention of Intraepithelial Neoplasia: An Important Target for Accelerated New Agent Development: Recommendations of the American Association for Cancer Research Task Force on the Treatment and Prevention of Intraepithelial Neoplasia. *Clin Cancer Res.* 2002 Feb 1;8(2):314–46.
5. Wu L, Qu X. Cancer biomarker detection: recent achievements and challenges. *Chemical Society Reviews.* 2015;44(10):2963–97.
6. Subramanian H, Pradhan P, Liu Y, Capoglu IR, Rogers JD, Roy HK, et al. Partial-wave microscopic spectroscopy detects subwavelength refractive index fluctuations: an application to cancer diagnosis. *Opt Lett, OL.* 2009 Feb 15;34(4):518–20.
7. Subramanian H, Pradhan P, Liu Y, Capoglu IR, Li X, Rogers JD, et al. Optical methodology for detecting histologically unapparent nanoscale consequences of genetic alterations in biological cells. *PNAS.* 2008 Dec 23;105(51):20118–23.
8. Adhikari P, Nagesh PKB, Alharthi F, Chauhan SC, Jaggi M, Yallapu MM, et al. Optical detection of the structural properties of tumor tissue generated by xenografting of drug-sensitive and drug-resistant cancer cells using partial wave spectroscopy (PWS). *Biomed Opt Express, BOE.* 2019 Dec 1;10(12):6422–31.
9. Subramanian H, Roy HK, Pradhan P, Goldberg MJ, Muldoon J, Brand RE, et al. Nanoscale Cellular Changes in Field Carcinogenesis Detected by Partial Wave Spectroscopy. *Cancer Res.* 2009 Jul 1;69(13):5357–63.
10. Almadadi HM, Nagesh PKB, Sahay P, Bhandari S, Eckstein EC, Jaggi M, et al. Optical study of chemotherapy efficiency in cancer treatment via intracellular structural disorder analysis using partial wave spectroscopy. *Journal of Biophotonics.* 2018;11(12):e201800056.
11. Adhikari P, Shukla PK, Alharthi F, Regmi B, Rao R, Pradhan P. Optical probing of nanostructural alterations of brain tissues by partial wave spectroscopy in chronic alcoholism. In: *Conference on Lasers and Electro-Optics (2020)*, paper AM3I4 [Internet]. Optical Society of America; 2020 [cited 2020 Aug 31]. p. AM3I.4. Available from: https://www.osapublishing.org/abstract.cfm?uri=CLEO_AT-2020-AM3I.4

12. Bhandari S, Shukla PK, Almagadi HM, Sahay P, Rao R, Pradhan P. Optical study of stress hormone-induced nanoscale structural alteration in brain using partial wave spectroscopic microscopy. *Journal of Biophotonics*. 2019;12(6):e201800002.
13. Sahay P, Almagadi HM, Ghimire HM, Skalli O, Pradhan P. Light localization properties of weakly disordered optical media using confocal microscopy: application to cancer detection. *Opt Express, OE*. 2017 Jun 26;25(13):15428–40.
14. Adhikari P, Hasan M, Sridhar V, Roy D, Pradhan P. Studying nanoscale structural alterations in cancer cells to evaluate ovarian cancer drug treatment, using transmission electron microscopy imaging. *Phys Biol*. 2020 Mar;17(3):036005.
15. Pradhan P, Damania D, Joshi HM, Turzhitsky V, Subramanian H, Roy HK, et al. Quantification of nanoscale density fluctuations by electron microscopy: probing cellular alterations in early carcinogenesis. *Phys Biol*. 2011 Mar;8(2):026012.
16. Adhikari P, Shukla PK, Hasan M, Alharthi F, Regmi B, Rao R, et al. Photonics study of probiotic treatment on brain cells exposed to chronic alcoholism using molecular specific nuclear light localization properties via confocal imaging. *arXiv:1912.11777*. 2019 Dec 25; Available from: <http://arxiv.org/abs/1912.11777>
17. Takikita M, Chung J-Y, Hewitt SM. Tissue microarrays enabling high-throughput molecular pathology. *Current Opinion in Biotechnology*. 2007 Aug 1;18(4):318–25.
18. Bubendorf L, Nocito A, Moch H, Sauter G. Tissue microarray (TMA) technology: miniaturized pathology archives for high-throughput in situ studies. *The Journal of Pathology*. 2001;195(1):72–9.
19. Adhikari P, Alharthi F, Pradhan P. Partial Wave Spectroscopy Detection of Cancer Stages using Tissue Microarrays (TMA) Samples. In: *Frontiers in Optics + Laser Science APS/DLS (2019)*, paper JW4A89. Optical Society of America; 2019. p. JW4A.89. Available from: <https://www.osapublishing.org/abstract.cfm?uri=FiO-2019-JW4A.89>
20. Sengupta B, Adhikari P, Mallet E, Havner R, Pradhan P. Spectroscopic Study on *Pseudomonas Aeruginosa* Biofilm in the Presence of the Aptamer-DNA Scaffolded Silver Nanoclusters. *Molecules*. 2020 Jan;25(16):3631.

21. Sauter G, Simon R, Hillan K. Tissue microarrays in drug discovery. *Nature Reviews Drug Discovery*. 2003 Dec;2(12):962–72.
22. McGuigan A, Kelly P, Turkington RC, Jones C, Coleman HG, McCain RS. Pancreatic cancer: A review of clinical diagnosis, epidemiology, treatment and outcomes. *World J Gastroenterol*. 2018 Nov 21;24(43):4846–61.
23. Sun Y-S, Zhao Z, Yang Z-N, Xu F, Lu H-J, Zhu Z-Y, et al. Risk Factors and Preventions of Breast Cancer. *Int J Biol Sci*. 2017 Nov 1;13(11):1387–97.
24. Kuipers EJ, Rösch T, Bretthauer M. Colorectal cancer screening—optimizing current strategies and new directions. *Nature Reviews Clinical Oncology*. 2013 Mar;10(3):130–42.
25. Killeen S, Mannion M, Devaney A, Winter DC. Complete mesocolic resection and extended lymphadenectomy for colon cancer: a systematic review. *Colorectal Disease*. 2014;16(8):577–94.
26. Cuzick J, Thorat MA, Andriole G, Brawley OW, Brown PH, Culig Z, et al. Prevention and early detection of prostate cancer. *The Lancet Oncology*. 2014 Oct 1;15(11):e484–92.
27. Litwin MS, Tan H-J. The Diagnosis and Treatment of Prostate Cancer: A Review. *JAMA*. 2017 Jun 27;317(24):2532–42.
28. Adhikari P, Binu AP, Bhandari S, Khan S, Jaggi M, Chauhan SC, et al. Optical detection of fractal dimensions of MUC13 stained pancreatic tissues for cancer diagnostics. arXiv:181210883. 2018 Dec 27; Available from: <http://arxiv.org/abs/1812.10883>
29. Bhandari S, Choudannavar S, Avery ER, Sahay P, Pradhan P. Detection of colon cancer stages via fractal dimension analysis of optical transmission imaging of tissue microarrays (TMA). *Biomed Phys Eng Express*. 2018 Oct;4(6):065020.