

# MIAFEx: An Attention-based Feature Extraction Method for Medical Image Classification

Oscar Ramos-Soto<sup>a</sup>, Jorge Ramos-Frutos<sup>b</sup>, Ezequiel Perez-Zarate<sup>c</sup>, Diego Oliva<sup>a,\*</sup>, Sandra E. Balderas-Mata<sup>a</sup>

<sup>a</sup>Departamento de Ingeniería Electro-Fotónica, Universidad de Guadalajara, CUCEI, Av. Revolución 1500, Guadalajara, 44430, Jalisco, México

<sup>b</sup>Posgrados, Centro de Innovación Aplicada en Tecnologías Competitivas, Omega 201, León, 37545, Guanajuato, México

<sup>c</sup>School of Computer Science and Technology, Zhejiang Gongshang University, Hangzhou, 310018, Zhejiang, China

---

## Abstract

Feature extraction techniques are crucial in medical image classification; however, classical feature extractors in addition to traditional machine learning classifiers often exhibit significant limitations in providing sufficient discriminative information for complex image sets. While Convolutional Neural Networks (CNNs) and Vision Transformer (ViT) have shown promise in feature extraction, they are prone to overfitting due to the inherent characteristics of medical imaging data, including small sample sizes or high intra-class variance. In this work, the Medical Image Attention-based Feature Extractor (MIAFEx) is proposed, a novel method that employs a learnable refinement mechanism to enhance the classification token within the Transformer encoder architecture. This mechanism adjusts the token based on learned weights, improving the extraction of salient features and enhancing the model's adaptability to the challenges presented by medical imaging data. The MIAFEx output features quality is compared against classical feature extractors using traditional and hybrid classifiers. Also, the performance of these features is compared against modern CNN and ViT models in classification tasks, demonstrating its superiority in accuracy and robustness across multiple complex classification medical imaging datasets. This advantage is particularly pronounced in scenarios with limited training data, where traditional and modern models often struggle to generalize effectively. The source code of this proposal can be found at [github.com/Oscar-RamosS/Medical-Image-Attention-based-Feature-Extractor-MIAFEx](https://github.com/Oscar-RamosS/Medical-Image-Attention-based-Feature-Extractor-MIAFEx).

**Keywords:** Medical image classification, Feature extraction techniques, Transformer encoder architecture

---

## 1. Introduction

Automated image classification in the medical field significantly improves diagnostics and healthcare [1] by separating image sets into distinct categories corresponding to various diseases or conditions. This process, usually done by artificial intelligence and machine learning (ML) systems, provides medical professionals a tool to identify diseases accurately [2] through imaging techniques such as Magnetic Resonance Imaging (MRI), Computed Tomography (CT) scans, among many others [3]. Additionally, these systems facilitate remote diagnostics, supporting telemedicine [4] and expanding access to remote healthcare areas. Nevertheless, access to large and labeled image datasets is often a significant challenge [5]. These sets are frequently limited in image quantity due to privacy concerns and the specialized nature of medical expertise required to annotate images [6]. For example, medical fields such as ophthalmology, radiology, and dermatology may consist of only a few hundred or thousand images, which is significantly less than the millions of images typically used to train general-purpose computer vision models [7]. Additionally, many medical images do not provide explicit visual features, making feature extraction challenging.

In computer vision, image feature extraction is a fundamental tool used to capture essential characteristics of an image in terms of numerical values [8], enabling classifiers to differentiate between classes or objects effectively by

---

\*Corresponding author

Email addresses: [oscar.ramos9279@alumnos.udg.mx](mailto:oscar.ramos9279@alumnos.udg.mx) (Oscar Ramos-Soto), [jramos.estudiantepicyt@ciatec.mx](mailto:jramos.estudiantepicyt@ciatec.mx) (Jorge Ramos-Frutos), [isaias.perez@alumnos.udg.mx](mailto:isaias.perez@alumnos.udg.mx) (Ezequiel Perez-Zarate), [diego.oliva@cucei.udg.mx](mailto:diego.oliva@cucei.udg.mx) (Diego Oliva), [sandra.balderas@academicos.udg.mx](mailto:sandra.balderas@academicos.udg.mx) (Sandra E. Balderas-Mata)

identifying and quantifying key visual attributes such as edges, textures, shapes, or color patterns. These features represent the image in a lower-dimensional space, allowing ML and hybrid models to process and classify images based on the extracted information. Effective feature extraction ensures that classifiers can generalize well to unseen data and avoid overfitting, especially in tasks with complex datasets or limited training data. When applied to medical datasets, classical feature extractors face significant problems due to the complexity of the images. These traditional techniques are specifically designed to capture simple local patterns like edges and gradients, but still struggle to detect the high-level features often needed in medical imaging tasks, such as detecting small lesions or understanding tissue structures [9]. Additionally, they cannot capture global context and relationships between different parts of an image, which is crucial for interpreting medical scans. These methods are also sensitive to noise and artifacts [10], and they do not scale well to the high-dimensional nature of medical data. As a result, these handcrafted methods often lead to poor performance in these feature classifications when compared to more modern, such as approaches like deep learning (DL).

In DL models such as Convolutional Neural Networks (CNNs) and Vision Transformers (ViT) [11, 12], overfitting and limited generalization are the main issues that arise when they are trained on tiny medical datasets. The latter issue leads the model to “memorize” the training images instead of learning patterns that may be applied to other datasets [13]. Because of this problem, a model may perform well on a certain dataset portion but poorly when used with additional patient images or in different imaging conditions. The CNNs rely heavily on large datasets to learn robust and meaningful features from the data. However, when training on small medical datasets, the model may learn small correlations or noise, leading to overfitting. Similarly, ViTs, which rely on self-attention mechanisms to capture global dependencies within an image, can struggle when insufficient data allows the model to learn the relationships between patches effectively. The nature of medical images complicates this issue, as they do not often provide easily identifiable features that a model can extract and learn from. Unlike natural images, where objects like cars, animals, or buildings have clear edges, shapes, and textures, as the ones in which modern techniques are trained, medical images can be highly abstract and require domain expertise to interpret.

This work presents the Medical Image Attention-based Feature Extractor (MIAFEx), a novel approach that enhances feature extraction by refining the classification token ([CLS] token) within the Transformer encoder. This refinement mechanism dynamically adjusts this token using learnable weights, allowing the model to prioritize salient features, crucial for medical image classification. The main contributions of this work can be summarized as follows:

- **Introduction of the MIAFEx framework:** A novel approach to medical image classification for complex, small, and imbalanced medical datasets.
- **Learnable Refinement mechanism:** MIAFEx introduces a dynamic and learnable refinement mechanism that adjusts the [CLS] token during training, enabling the model to focus on the most relevant features for classification improving model performance.
- **Comparative analysis:** The proposed method is compared against classical feature extraction techniques combined with ML classifiers, emphasizing its effectiveness.
- **Extensive experimental validation:** The obtained results were evaluated across diverse medical imaging datasets, presenting superior performance compared to traditional and modern methods like CNNs and ViT, especially on smaller datasets.

The remainder of this paper is organized as follows: Section 2 reviews related work relevant to this study, while Section 3 provides a detailed explanation of the MIAFEx framework, detailing its structure and functionality. Section 4 outlines the experimental framework designed to evaluate the performance of MIAFEx, including a description of the dataset and the techniques employed for comparative analysis. Section 5 presents comprehensive results from the evaluation, highlighting the method’s effectiveness through rigorous comparison. Finally, Section 6 summarizes the findings and conclusions of this work, along with potential directions for future research.

## 2. Related work

In recent decades, feature extraction techniques have played an important role in medical image classification for disease detection. Classical methods for feature extraction, such as Scale-Invariant Feature Transform (SIFT) [14],

Local Binary Patterns (LBP) [15], and Histogram of Oriented Gradients (HOG) [16], have long been used in traditional computer vision and also in the medical area [17]. The performance of capturing the most relevant image features highly impacts the classifier’s accuracy. Numerous approaches have been developed for a wide range of medical imaging applications using these classical techniques among many others. Some of the most relevant approaches are presented below.

### 2.1. Classical and hybrid approaches

In 2018, Alhindi et al. [18] compared LBP, HOG, and deep features for histopathological image classification, finding that the best performance was achieved using LBP combined with a Support Vector Machine (SVM), with an accuracy of 90.52% across 20 classes. That same year, Liebgott et al. publicly released a robust toolbox called ImFEATbox [19], providing MATLAB users with a comprehensive set of local and global feature descriptors, including geometrical, intensity, region, texture, and moment-based features. ImFEATbox was tested on MRI prostate cancer and FDG-PET/CT lung cancer images, performing statistical analyses using an SVM. Concurrently, Raj et al. [20] utilized both the Gray-level Co-occurrence Matrix (GLCM) and Gray-level Run Length Matrix (GLRLM) to extract features from three medical datasets to differentiate between Alzheimer’s disease and various cancers, selecting 15 features for classification using the metaheuristic-based opposition crow search (OCS).

In 2021, Aswiga et al. [21] tackled the issue of limited datasets by introducing Feature Extraction Based Transfer Learning (FETL), which combines three different feature extraction techniques to enhance basic multilevel transfer learning (MLTL) for mammography datasets, classifying benign, malignant, and normal images.

Several proposals also demonstrate successful hybridization strategies to address feature extraction challenges in medical image datasets. For instance, metaheuristic optimization [22] has been widely applied to reduce feature complexity and aid in feature selection. In 2016, Nagarajan et al. [23] proposed a hybrid genetic algorithm using branch and bound techniques and the artificial bee colony algorithm, applied to thyroid, breast cancer, and brain tumor images. Their approach incorporated the Intrinsic Pattern Extraction Algorithm, Texton-based Contour Gradient Extraction (TCGR), and SIFT for robust feature extraction.

In 2018, Echegaray et al. [24] introduced the Quantitative Image Feature Engine (QIFE) for volumetric medical image feature extraction using multiprocessor parallelization, primarily leveraging Haralick features and GLCM applied to DICOM files. In 2022, Kuwil [25] developed the Feature Extraction Based on Region of Mines (FE\_mines), which extracts features from the red, green, and blue channels based on statistical measurements such as mean, standard deviation, and coefficient of variance. It was tested on MRI, X-ray, and eye fundus images, achieving high performance across all types. Also in 2023, Sharma et al. [26] hybridized HOG with a variant of ResNet-50 for brain tumor detection in MRI images, achieving an accuracy of 88%, outperforming several other techniques. That same year, Narayan et al. [27] introduced FuzzyNet, a model for image classification that uses GLCM features and particle swarm optimization to perform binary differentiation in musculoskeletal radiographs, incorporating noise reduction and contrast enhancement before model implementation.

### 2.2. CNN and ViT approaches

On the other hand, DL-based methods such as convolutional layers in CNNs and self-attention mechanisms in ViT have gained interest for feature extraction in modern models, hence the number of papers regarding the classification of medical images using CNN or ViT models and variants has highly increased [28, 29, 30, 31, 32].

One of the most relevant works is MedViT, presented by Manzari et al. [33]. This proposal introduces a CNN-Transformer hybrid model designed to reduce model complexity while enhancing high-level information by considering feature variance and mean on large-scale datasets, such as those in MedMNIST-2D. In the same year, Ding et al. developed FTransCNN [34], which combines fuzzy logic, CNN, and transformer architectures to enhance local details and eliminate irrelevant regions. Their model incorporates a fuzzy attention fusion module (FAFM) to capture both high and low-level features in chest X-ray and endoscopy images, achieving high performance on both datasets. More recently, in 2024, Huo et al. introduced the HiFuse model [35], which employs a parallel hierarchical structure, an adaptive hierarchical feature fusion (HFF) block, and an inverted residual multi-layer perceptron (IRMLP) to build a robust model that avoids introducing noise. HiFuse was tested on various image types, including skin lesions, endoscopic, chest CT, and microscopic images. In the same year, Yue and Li designed the MedMamba [36], mainly based on the hybrid basic block named SS-Conv-SSM which implies the use of convolutional layers for local feature extraction. It was tested on sixteen datasets with a total of 411,007 images across ten different imaging modalities.

As observed, there are several previously proposed methods related to medical image feature extraction and classification. However, most of them are tested on large datasets or use several feature extractors, which improves the classification performance in both classical, hybrid, and DL approaches. Also, the best-performing ones require large computational resources to obtain great results, making difficult clinical implementation.

### 3. MIAFEx design

In this section, the MIAFEx is described in detail, emphasizing the refinement mechanism. In a general way, this approach processes input train images, dividing them into patches and extracting feature classification embeddings [CLS] through a transformer encoder using the ViT architecture. Then, this [CLS] token enters the refinement mechanism, first multiplying it with learnable refinement weights to prioritize relevant features. This refined token is passed through a fully connected layer, and a softmax function processes the output to produce class probabilities. The model is trained using cross-entropy loss, and during backpropagation, both the refinement weights and the model parameters are updated to improve classification performance. This is defined as the training part. Then, the trained model is used for a test dataset refined feature extraction, for a later feature selection using any classifier, named as the inference step. The above-described general MIAFEx process is summarized in Fig. 1. A more detailed explanation is presented below.

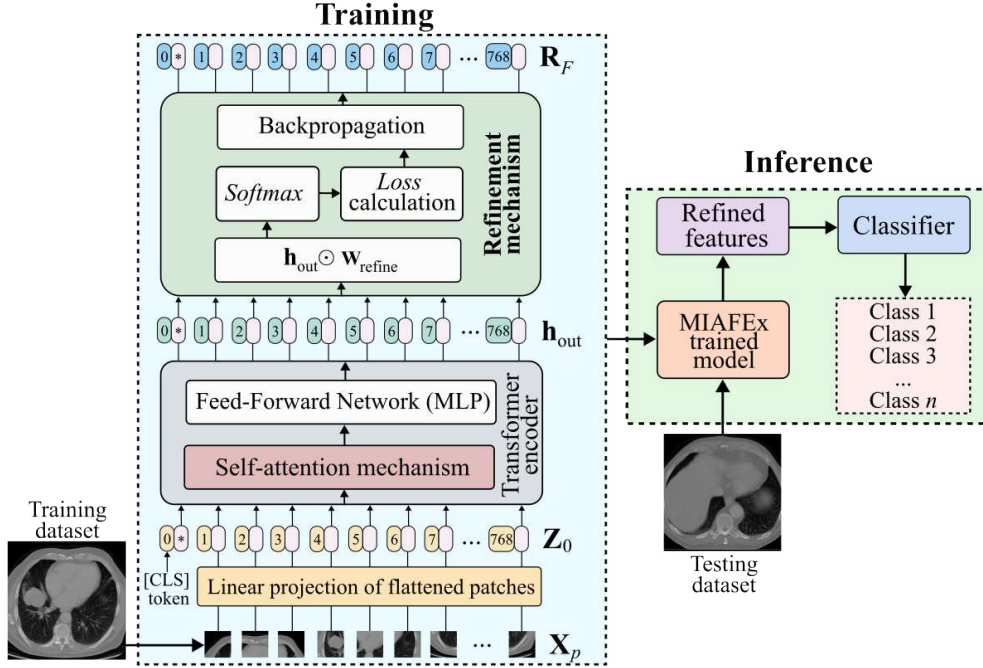


Figure 1: General diagram of the MIAFEx.

#### 3.1. Patch embedding

In the ViT model [37] (whose core element is the transformer encoder), the input image  $\mathbf{X} \in \mathbb{R}^{H \times W \times C}$  (where  $H$ ,  $W$ , and  $C$  represent the height, width, and number of channels, respectively) is divided into fixed-size patches. Each patch is flattened and linearly projected into a  $D$ -dimensional vector. Let  $\mathbf{X}_p \in \mathbb{R}^{N \times D}$  represent the sequence of  $N$  patch embeddings, where  $N = \frac{H \cdot W}{P^2}$  is the total number of patches, and  $P \times P$  is the patch size.

In addition to the patch embeddings, a learnable [CLS] token is prepended to the sequence, which serves as a summary representation for the entire image. Mathematically, the input to the transformer encoder is:

$$\mathbf{Z}_0 = [\text{CLS}; \mathbf{X}_p] + \mathbf{E}_{\text{pos}} \quad (1)$$

where  $\mathbf{Z}_0 \in \mathbb{R}^{(N+1) \times D}$  is the initial input, and  $\mathbf{E}_{\text{pos}}$  represents position embeddings that encode the location of each patch.

In this approach, the selected input image size is  $224 \times 224 \times 3$  (height, width, and RGB channels). Then, the image is divided into patches of size  $16 \times 16$  and each patch is treated as a token, similar to how tokens are used in natural language processing with transformers. After flattening each patch, a vector of size  $P^2 \times C$  is obtained. In this case, the size of each flattened patch is  $16 \times 16 \times 3 = 768$ . Each of these flattened patches is then linearly projected into a  $D$ -dimensional space, in ViT’s base version. This projection ensures that all patches have a consistent embedding dimension that the transformer can process.

### 3.2. Transformer encoder

The transformer encoder consists of  $L$  layers, each composed of a multi-head self-attention mechanism and a Feed-forward Network, in this case, a multi-layer perceptron (MLP). The [CLS] token and the patch embeddings are updated in each layer based on interactions between all tokens. Let  $\mathbf{Z}_L \in \mathbb{R}^{(N+1) \times D}$  represent the output of the  $l$ -th transformer layer. After processing through all  $L$  layers, the output corresponding to the [CLS] token is extracted as the global representation of the image:

$$\mathbf{Z}_L = [\mathbf{h}_{\text{out}}; \mathbf{X}_{p,\text{out}}] \quad (2)$$

where  $\mathbf{h}_{\text{out}}$  is the final output of the [CLS] token after it has interacted with all the patch tokens through the transformer layers.

The processed [CLS] token, from now on referred to in this document as  $\mathbf{h}_{\text{out}}$ , works as a summary token that gathers global information from all patches via the self-attention mechanism. It serves as both an input (to initiate the encoding process) and as an output, representing the holistic image features. The  $\mathbf{h}_{\text{out}}$  token is passed to the final classification head or further refined using additional mechanisms to optimize performance.

### 3.3. Refinement Mechanism

After passing through  $L$  transformer encoder layers, the output corresponding to the  $\mathbf{h}_{\text{out}}$  token is extracted from the last layer, mathematically defined as:

$$\mathbf{h}_{\text{out}} = [h_1, h_2, \dots, h_D] \quad (3)$$

where  $D$  is the dimensionality of the token, in this approach  $D = 768$ , each  $h_i$  represents a scalar feature corresponding to the  $i$ -th dimension of the  $\mathbf{h}_{\text{out}}$  token.

In the refinement mechanism, a set of learnable weights  $\mathbf{w}_{\text{refine}}$  is introduced, which is a vector of the same dimensionality as the  $\mathbf{h}_{\text{out}}$ . These weights are initialized randomly and are trained along with the rest of the model. The refinement weights can be represented as:

$$\mathbf{w}_{\text{refine}} = [w_1, w_2, \dots, w_D] \quad (4)$$

Each  $w_i$  is a scalar weight corresponding to the  $i$ -th dimension of the  $\mathbf{h}_{\text{out}}$  token. These weights allow the model to amplify, attenuate, or ignore certain features in the  $\mathbf{h}_{\text{out}}$  during training. The refinement process involves applying an element-wise multiplication between the  $\mathbf{h}_{\text{out}}$  and the refinement weights  $\mathbf{w}_{\text{refine}}$ . This operation modifies each dimension of the  $\mathbf{h}_{\text{out}}$  token according to the learned importance of that feature. Mathematically, this is expressed as:

$$\mathbf{R}_0 = \mathbf{h}_{\text{out}} \odot \mathbf{w}_{\text{refine}} \quad (5)$$

where  $\odot$  represents element-wise multiplication. In expanded form, this becomes:

$$\mathbf{R}_0 = [h_1 \cdot w_1, h_2 \cdot w_2, \dots, h_D \cdot w_D] \quad (6)$$

Each element of the  $\mathbf{h}_{\text{out}}$  token is scaled by its corresponding refinement weight in  $\mathbf{w}_{\text{refine}}$ . The refinement weights allow the model to prioritize certain features based on their relevance to the task. This refined feature vector  $\mathbf{R}_0$  is passed to a fully connected layer for classification:

$$\hat{y} = \text{softmax}(a \cdot \mathbf{R}_0 + b) \quad (7)$$

where  $a$  and  $b$  are the weights and bias of the classifier, and  $\hat{y}$  represents the predicted class probabilities.

To train the model, the predicted class probabilities  $\hat{y}$  are compared to the true labels using the cross-entropy loss function, defined as:

$$\mathcal{L}_{\text{CE}}(\hat{y}, y) = - \sum_{i=1}^C y_i \log(\hat{y}_i) \quad (8)$$

where  $y$  is the one-hot encoded true label,  $C$  is the number of classes, and  $\hat{y}_i$  is the predicted probability for class  $i$ . This loss function penalizes the model based on how far the predicted probabilities are from the true labels. After computing the loss, backpropagation is performed to update the learnable parameters of the model, including the refinement weights  $\mathbf{w}_{\text{refine}}$ , as well as the weights and biases in the classifier. Through multiple training iterations, this process allows the model to learn and refine the features extracted from the  $\mathbf{h}_{\text{out}}$  token, improving classification accuracy over time. The final refined hidden state,  $\mathbf{R}_F$ , now represents the final feature vector extracted.

The refinement mechanism can be understood as a process that adjusts the contribution of each feature dimension in the  $\mathbf{h}_{\text{out}}$  token. If a refinement weight  $w_i$  is close to 0, the corresponding feature  $h_i$  will be suppressed. Conversely, if  $w_i > 1$ , the feature  $h_i$  will be amplified. The key idea behind it is to allow the model to dynamically adjust the importance of different token dimensions. Each dimension in the hidden state represents a specific feature of the input image, and not all features are equally relevant to the classification task. By learning the refinement weights, the model can down-weight irrelevant features and up-weight the important ones.

The refinement mechanism plays a crucial role in adjusting the feature representation of the transformer encoder output, ensuring that the most relevant features for the classification task are emphasized, while less important features are down-weighted. This improves the overall performance of the Transformer encoder by allowing the model to dynamically refine the learned features during training.

## 4. Experimental framework

In this section, the selected datasets for the MIAFEx testing are presented, followed by the description of the ML classifiers and DL used for comparison. Also, the classification performance metrics and the experimental configuration for the model test are detailed.

### 4.1. Datasets

To evaluate the efficiency of the MIAFEx framework, a selection of diverse datasets was chosen, each representing unique challenges in medical image analysis. These datasets were chosen based on their varying image acquisition methods, dataset sizes, and the visual complexity of the images. Below, we present the details of the datasets used in the study.

#### 4.1.1. Histological biopsy

The histological biopsy is a widely used microscopy-based imaging study to observe different tissues at a cell level. The chosen dataset<sup>1</sup> includes images from three classes namely chronic lymphocytic leukemia (CLL), follicular lymphoma (FL), and mantle cell lymphoma (MCL). Images were acquired with an AxioCam MR5 CCD camera, a Zeiss Axioscope white light microscope, and 20x objective. 57 training images per class of  $1040 \times 1388$  pixels were taken which were divided into 30 mosaics of  $208 \times 231$  pixels from each image giving a total of 1710 images per class. 56, 82, and 65 images were used in the CLL, FL, and MCL testing, respectively. Images of the three classes mentioned are shown in Fig. 2.

<sup>1</sup><https://www.kaggle.com/datasets/andrewmvd/malignant-lymphoma-classification>

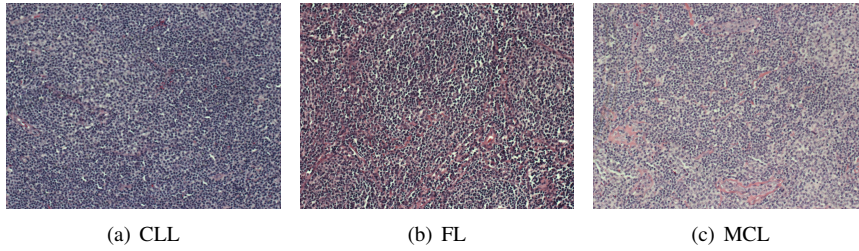


Figure 2: Histological biopsy images.

#### 4.1.2. Ocular alignment

Strabismus is a condition where the eyes are not aligned and can cause the brain to ignore signals from the eye or not perceive depth in the environment. In this work, the dataset selected for strabismus<sup>2</sup> consists of four distinct classes, each representing a specific type of ocular misalignment, along with a fifth class for correctly aligned eyes. The first is Esotropia which is shown when the eyes deviate inwards (100 images). Exotropia which causes the eyes to deviate outwards (104 images). The third is Hypertropia which causes the eyes to deviate upwards (104 images). The last is Hypotropia where the eyes deviate downwards (93 images). The fifth classification is where the eyes are aligned correctly (110 images). The image dataset consists of 509 total images with different sizes. Figure 3 illustrates images representing the five specified classes.

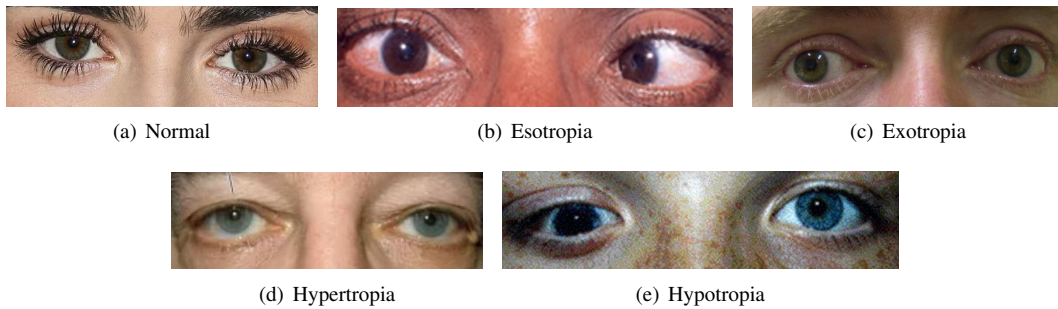


Figure 3: Ocular alignment images.

#### 4.1.3. Eye fundus

By using an ophthalmoscope, it is possible to observe the inner part of the human eye, specifically the retina, which plays a vital role in the eye's sensorial function. This study is known as eye fundus imaging. The dataset used<sup>3</sup> contains eye fundus images of some diseases that affect this organ and that increase the risk of human beings going blind. There are four categories in the dataset: normal, cataract, glaucoma, and retinal disease. There are 300 images of the normal class and 300 images distributed in hundredths in each disease class, adding one more to the glaucoma class. The sizes of the images are varied. Images corresponding to the four mentioned classes are displayed in Fig. 4.

#### 4.1.4. Ultrasound breast cancer

Breast cancer has gained significant attention in recent times due to its high mortality rate and the increasing number of reported cases. Using the ultrasound imaging technique makes it possible to observe the tissue distribution for cancer visual detection, making it an early detection alternative to diminish the public health impact. The dataset<sup>4</sup>

<sup>2</sup><https://www.kaggle.com/datasets/ananthamoorthy/strabismus>

<sup>3</sup><https://www.kaggle.com/datasets/jr2ngb/cataractdataset>

<sup>4</sup><https://www.kaggle.com/datasets/sabahearak/breast-ultrasound-images-dataset>

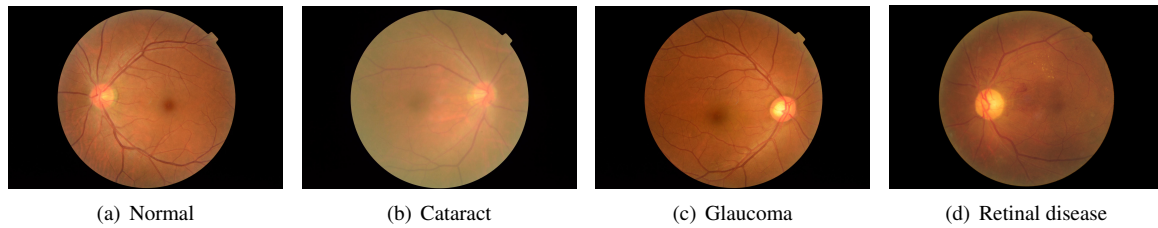


Figure 4: Eye fundus images.

used in this work contains 780 images with three categories: benign with 442 images, malignant with 206, and normal with 132. The scans were collected from 600 women between 25 and 75 years old. It is a highly unbalanced dataset with different image sizes, having an average of  $500 \times 500$  pixels [38]. Figure 5 showcases examples from each of the three described classes.

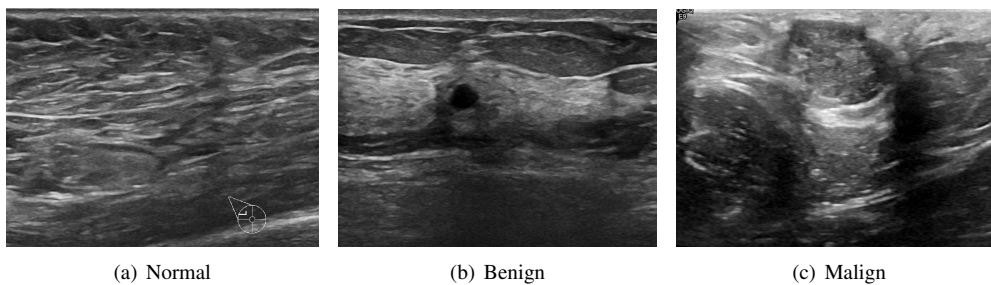


Figure 5: Breast ultrasound images.

#### 4.1.5. Chest CT

Chest CT scans play a relevant role in diagnosing a wide range of thoracic diseases, from infections to malignancies. By analyzing those scans, it is possible to detect diseases in the chest region, including pneumonia and cancer. The selected chest CT dataset <sup>5</sup> contains 967 images across normal and three cancer types: adenocarcinoma, large-cell carcinoma, and squamous-cell carcinoma. Figure 6 provides a visual representation of the four highlighted classes.

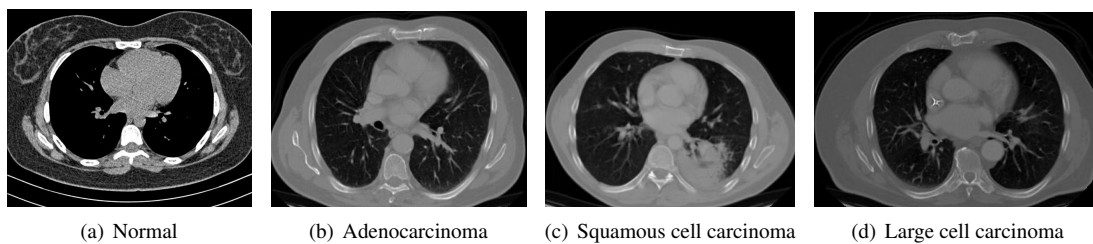


Figure 6: Chest CT scans.

#### 4.1.6. Brain MRI

Brain tumors pose significant health challenges, often impacting critical functions such as vision, balance, and cognition. Early detection is crucial for improving patient outcomes and quality of life. Through MRI scans, different

<sup>5</sup><https://www.kaggle.com/datasets/mohamedhanyyy/chest-ctscan-images>



conditions of the brain can be visually detected. The selected brain tumor dataset <sup>6</sup> contains 3,362 images across four categories: glioma, meningioma, pituitary tumors, and normal brains. Images illustrating the three aforementioned classes can be found in Fig. 7.

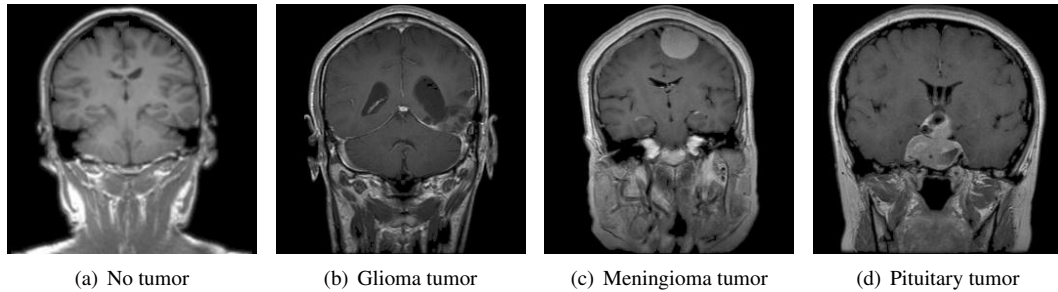


Figure 7: Brain MRI scans.

#### 4.1.7. Gastrointestinal endoscopy

Endoscopies are used to detect diseases in the human digestive system. Images from inside the gastrointestinal tract can be used to help doctors detect diseases early. The used dataset <sup>7</sup> contains eight image categories of the digestive system obtained through the endoscopy imaging technique, as shown in Fig. 8. There are a total of 6000 images that can be used in training and testing machine learning algorithms.

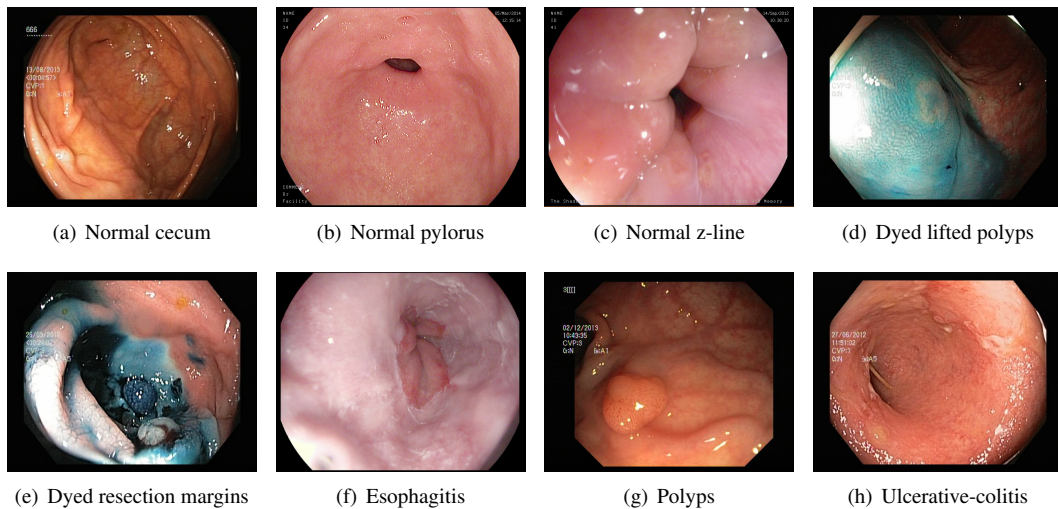


Figure 8: Gastrointestinal endoscopy images.

Table 1 provides a detailed summary of the datasets used in this study, highlighting the total number of images in each dataset, the distribution between training and testing sets, and the specific classes represented. Each dataset corresponds to a particular medical imaging domain with distinct classes relevant to diagnosing specific conditions. Also, Fig. 9 presents a representative image from each dataset, allowing for a visual comparison of the diverse tones, patterns, and textures present across the datasets. Such diversity in visual characteristics highlights the need for a robust model that can handle all image characteristics.

<sup>6</sup><https://www.kaggle.com/datasets/sami009mr/brain-tumor-dataset>

<sup>7</sup><https://www.kaggle.com/datasets/abdallahwagih/kvasir-dataset-for-classification-and-segmentation>

Table 1: Selected datasets distribution and classes.

Dataset	Total images	Train images	Test images	Classes
Histological biopsy	374	298	76	Chronic lymphocytic leukemia Follicular lymphoma Mantle cell lymphoma
Ocular alignment	509	405	104	Normal Esotropia Exotropia Hypertropia Hypotropia
Eye fundus	601	480	121	Normal Cataract Glaucoma Retinal disease
Breast ultrasound	780	619	161	Normal Benign Malign
Chest CT	967	613	354	Normal Adenocarcinoma Squamous cell carcinoma Large cell carcinoma
Brain MRI	3362	2688	674	No tumor Glioma tumor Meningioma tumor Pituitary tumor
Gastrointestinal endoscopy	4000	3200	800	Normal cecum Normal pylorus Normal z-line Dyed lifted polyps Dyed resection margins Esophagitis Polyps Ulcerative-colitis

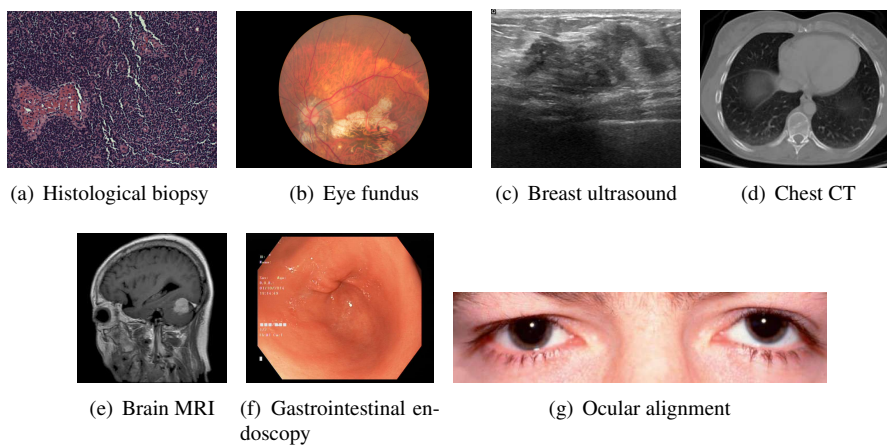


Figure 9: Example images of each dataset.

#### 4.2. Classical feature extractors

A variety of classical methods for feature extraction are employed to benchmark and compare the performance of the MIAFEx framework. Below, a detailed overview of the selected techniques is provided, highlighting their key characteristics and relevance to the comparison.

- **Histogram of Oriented Gradients (HOG)**

The Histogram of Oriented Gradients (HOG) [16] operates by dividing an image into blocks, computing the gradient magnitude and direction at each pixel, and constructing histograms of gradient orientations for these blocks. These histograms are normalized across blocks to achieve robustness against illumination changes and shadowing. The HOG technique is effective for detecting edges and shapes, making it popular in applications like object detection. However, its sensitivity to noise and limited ability to capture global image context reduce its effectiveness in complex scenarios, such as medical imaging, where subtle variations are critical.

- **Scale-Invariant Feature Transform (SIFT)**

The Scale-Invariant Feature Transform (SIFT) [14] identifies key points in an image that remain consistent across changes in scale, rotation, and illumination. It achieves this by detecting extrema in the Difference of Gaussians (DoG) across multiple scales, assigning gradient-based orientations, and generating descriptors that summarize local image features. These descriptors are robust to transformations and are widely used in texture classification and object recognition. Despite its strength in analyzing local features, SIFT's high computational cost and inability to capture global patterns limit its application in medical imaging tasks that often require understanding broader contextual relationships.

- **Local Binary Pattern (LBP)**

Local Binary Patterns (LBP) [15] encode local texture information by comparing pixel intensities in a neighborhood and creating a binary pattern for each pixel. The resulting patterns are aggregated into histograms, which serve as texture descriptors. LBP is computationally efficient and rotation-invariant, making it suitable for simple texture-based tasks. However, its sensitivity to noise and variations in illumination, along with its focus on local regions, makes it less robust for medical images that require capturing fine-grained structural features over larger contexts.

- **Haralick Texture Features (HTFs)**

Haralick Texture Features (HTFs) [39] leverage the gray-level co-occurrence matrix (GLCM) to compute statistical measures, such as contrast, homogeneity, and entropy, that characterize spatial relationships between pixel intensities. These features are widely used in texture analysis for applications like cancer detection and tissue classification. While HTFs provide valuable insights into textural patterns, their computational demands and reliance on predefined spatial relationships make them less adaptable to diverse datasets and imaging conditions, as encountered in medical contexts.

- **Gabor Filter (GF)**

Gabor Filters [40] combines spatial and frequency domain analysis to capture textures and edge information. Each Gabor filter is defined by a Gaussian envelope modulating a sinusoidal wave, and a filter bank with multiple scales and orientations is used to extract localized features. Gabor filters excel in tasks like fingerprint recognition and texture segmentation, where their ability to capture directional features is crucial. However, they are computationally intensive, sensitive to parameter tuning, and may produce redundant information in complex or noisy images, limiting their efficiency in dynamic medical imaging scenarios.

#### 4.3. Tested classifiers

Once the MIAFEx features were extracted from the datasets, they were classified using ML techniques. For comparison purposes, DL models (CNNs and the ViT) are used to perform the classification task on the same dataset and observe the performance of the MIAFEx features alongside different classifiers. These techniques and models are listed below.

#### 4.3.1. Machine learning (ML) classifiers

- **Logistic regression (LR)**

Logistic regression [41] is a statistical method used for binary classification tasks. It models the probability that a given input belongs to a specific class by applying the logistic function to a linear combination of the input features. Despite its simplicity, LR is widely used for its effectiveness, especially in binary classification problems.

- **Random forest (RF)**

Random Forest [42] is an ensemble learning method that constructs multiple decision trees during training and merges their predictions to improve accuracy and reduce overfitting. Each tree is trained on a different random subset of the data, and predictions are made based on the majority vote (classification) or average (regression) of all trees.

- **Support vector machine (SVM)**

Support Vector Machine (SVM) [43] is a powerful supervised learning algorithm used for classification and regression tasks. SVM aims to find the optimal hyperplane that maximizes the margin between different classes in the feature space. It is particularly effective for high-dimensional data and can handle both linear and non-linear classification using kernel functions.

- **Extreme gradient boosting (XGBoost)**

XGBoost [44] is an efficient and scalable implementation of gradient boosting, an ensemble technique that builds multiple weak learners (typically decision trees) in sequence. Each tree corrects the errors of the previous one, and the final model combines all trees to make more accurate predictions. XGBoost is known for its high performance and speed, particularly in structured data tasks.

- **Wrapper-based feature selection (WFS) and metaheuristics**

Wrapper-based feature selection is a technique that evaluates the performance of an (ML) model using different subsets of features to identify the most relevant ones [45, 46]. It “wraps” the feature selection process around the learning algorithm to optimize the selected subset. Metaheuristic algorithms are often used to efficiently explore the search space of feature subsets, especially when dealing with large datasets, to improve the overall model’s performance.

#### 4.3.2. Deep learning (DL) models

- **MobileNet-V2**

MobileNet-V2 [47] is a lightweight CNN designed for mobile and edge devices, intending to optimize both performance and efficiency. It uses depthwise separable convolutions to reduce the number of parameters and computations while maintaining accuracy. MobileNet-V2 introduces linear bottleneck layers and inverted residuals, allowing for effective feature extraction with minimal latency, making it suitable for real-time applications.

- **DenseNet-161**

DenseNet-161 [48] is a deep CNN that enhances feature propagation and reuse through densely connected layers. In this architecture, each layer receives input from all previous layers, which improves gradient flow and reduces the risk of vanishing gradients. DenseNet-161 consists of 161 layers, allowing for more efficient training and higher accuracy, particularly in image classification tasks.

- **ResNet-50**

ResNet-50 [49] is a widely used deep residual network that tackles the vanishing gradient problem through skip connections, allowing gradients to flow through the network more effectively. Comprising 50 layers, ResNet-50 facilitates the training of very deep networks while maintaining high performance. Its architecture also enables the reuse of features, making it effective for various image recognition tasks and a popular choice for transfer learning.

- **Vision Transformer (ViT)**

Vision Transformer (ViT) [37] is a revolutionary model that applies transformer architecture which was originally designed for natural language processing. Instead of using convolutional layers, ViT divides images into patches and processes them as sequences, leveraging self-attention mechanisms to capture global dependencies and context. This approach has proven to be highly effective on large-scale datasets, demonstrating that ViT usually outperforms traditional CNNs in vision tasks.

#### 4.4. Performance metrics

Evaluating classification algorithms is a fundamental part of determining whether the classification problem they solve is being solved. To evaluate the algorithms in the classification task, the Accuracy, Precision, Recall, and F1-score metrics are used.

Accuracy measures how many times the algorithm gets its predictions right out of the total number of records. Equation 9 is used to determine the accuracy of ML algorithms.

$$\text{Accuracy} = \frac{\text{TP} + \text{TN}}{\text{TP} + \text{TN} + \text{FP} + \text{FN}} \quad (9)$$

where TP represents the number of positive cases correctly identified as positive, TN denotes the number of negative cases correctly identified as negative, FN indicates the number of positive cases mistakenly classified as negative, and FP refers to the number of negative cases incorrectly classified as positive.

On the other hand, Precision measures the algorithm’s ability to predict true positives against the total number of positive records. If this value is detected high, the algorithm is sensitive to true positives and will be effective in detecting any disease. Equation 10 shows the computation of the precision.

$$\text{Precision} = \frac{\text{TP}}{\text{TP} + \text{FN}} \quad (10)$$

Equation 11 is used to obtain the Recall of a classification algorithm. The recall measures the proportion of all true positives that were correctly classified as positives. This metric is also known as the true positive rate.

$$\text{Recall} = \frac{\text{TP}}{\text{TP} + \text{FN}} \quad (11)$$

Finally, the F1-score is a metric that allows measuring the quality of a model to predict imbalanced datasets. It is computed using Eq. 12.

$$F1\text{-score} = 2 \times \frac{\text{Precision} \times \text{Recall}}{\text{Precision} + \text{Recall}} \quad (12)$$

Since this is a multiclass analysis, the weighted average of these metrics is used to provide a single comprehensive value that accounts for the performance across all classes. The weighted average ensures that the contribution of each class to the overall metric is proportional to the number of true instances in that class, hence preventing skewed results due to class imbalances. The weighted average for a metric  $M$  across all classes can be calculated using the formula:

$$M_{\text{weighted}} = \frac{\sum_{i=1}^n N_i \cdot M_i}{\sum_{i=1}^n N_i} \quad (13)$$

where  $M_i$  is the metric value for class  $i$ ,  $N_i$  is the number of true instances in class, and  $n$  is the total number of classes.

#### 4.5. Experimental setup

Table 2 provides an overview of the parameter configurations for the feature extractors employed in the study, which include HOG, SIFT, LBP, HTFs, and GF. It details key parameters such as the number of orientations, cell sizes, and other specific settings for each feature extraction method.

Table 3 presents the configuration for the classifiers used, which include SVM, RF, LR, and XGBoost. This table highlights important parameters such as regularization strength, kernel types, and the number of estimators for each

classifier. These tables ensure a clear understanding of the settings used for both feature extraction and classification in the experiment.

The experimental configuration of the WFS method was performed by the K-nearest neighbors (KNN) algorithm within the following metaheuristic algorithms: Particle Swarm Optimization (PSO) [50], Differential Evolution (DE) [51], and the Genetic Algorithm (GA) [52]. Each metaheuristic algorithm was applied with the number of particles set to 30 and a maximum of 200 iterations.

Regarding the MIAFEx and all DL models, the same configuration was applied. The training process ran for 10 epochs using the Nesterov-accelerated Adaptive Moment Estimation (Nadam) optimizer, with a learning rate of  $1 \times 10^{-4}$  [53], and the loss was computed using the cross-entropy loss function [54]. To accelerate convergence and improve model performance, transfer learning [55] was employed across all models. For MIAFEx and ViT training, pre-trained weights from the *ImageNet-21k* dataset [56, 57] (ViT-base-patch16-224) were utilized [58]. Meanwhile, for the other CNNs, transfer learning was performed using pre-trained weights from the *ImageNet-1K* dataset [59]. A batch size of 8 was used during training for all models to ensure consistent input size across experiments.

Table 2: Summary of feature extractor parameter configurations.

Feature Extractor	Parameter	Value	Description
HOG	Orientations	9	Number of bins in the histogram.
	Pixels per cell	$8 \times 8$	Size of each cell in pixels.
	Cells per block	$2 \times 2$	Number of cells per block.
	Block normalization	L2-Hys	Normalization method for histograms.
SIFT	Keypoint detector	SIFT	Algorithm for detecting keypoints.
	Descriptor length	Variable (padded to max)	Length of the descriptor vector.
LBP	Radius	1	Radius of the neighborhood.
	Points	$8 \times$ radius	Number of sample points.
	Method	Uniform	Uniform patterns for histogram computation.
HTFs	Distances	1	Pixel distances for the GLCM computation.
	Angles	$\{0, \pi/4, \pi/2, 3\pi/4\}$	Directions for computing GLCM.
Gabor Filter	Kernel size	$21 \times 21$	Size of the Gabor kernel.
	Scales ( $\sigma$ )	$\{1, 3\}$	Determines the width of the Gabor filter.
	Orientations ( $\theta$ )	4 (0 to $\pi$ )	Number of orientations to apply.
	Wavelength ( $\lambda$ )	$\pi/4, \pi/2$	Wavelengths of the sinusoidal factor.

Table 3: Summary of classifier parameter configurations.

Classifier	Parameter	Value	Description
SVM	C	1	Regularization parameter.
	kernel	Radial basis function	Specifies the kernel type.
	degree	3	Degree of the polynomial kernel function.
RF	Estimators	100	The number of trees in the forest.
	Criterion	Gini	The function to measure the quality of a split.
	Random state	42	Seed used by the random number generator.
LR	C	1.0	Inverse regularization strength.
	Solver	LBFGS	Algorithm to use in optimization.
	Max iterations	1000	Maximum number of iterations for solver.
XGBoost	Random state	42	Seed used by the random number generator.
	Estimators	100	Number of boosting rounds.
	Learning rate	0.1	Step size at each iteration.
	Max depth	6	Maximum depth of the tree.
	Random state	42	Seed used by the random number generator.

## 5. Results

This section presents the experimental results across the different medical imaging datasets described above. First, MIAFEx-extracted features are compared with classical feature extractors across a range of ML classifiers to evaluate relative performance. Next, the study assesses MIAFEx’s effectiveness in comparison to DL models, examining its behavior across diverse datasets to determine its robustness. Finally, an analysis of how classification performance varies with dataset size is provided, offering insights into the scalability and adaptability of each model.

### 5.1. Classical feature extractors and MIAFEx performance with ML classifiers

The performance of the MIAFEx was evaluated in conjunction with various classifiers, and its efficacy in feature extraction was compared. The feature extraction techniques considered for comparison were HOG, SIFT, LBP, HTFs, and GF, and the classifiers tested include SVM, RF, LR, XGBoost, and evolutionary optimization techniques (WFS-PSO, WFS-DE, and WFS-GA). In Fig. 10, the accuracy heatmaps of all the combinations of feature extractor, classifier, and dataset are presented. Due to its extensive length, complete tables presenting the analysis of performance across all metrics are included in Appendix A for clarity and to maintain the flow of the main document.

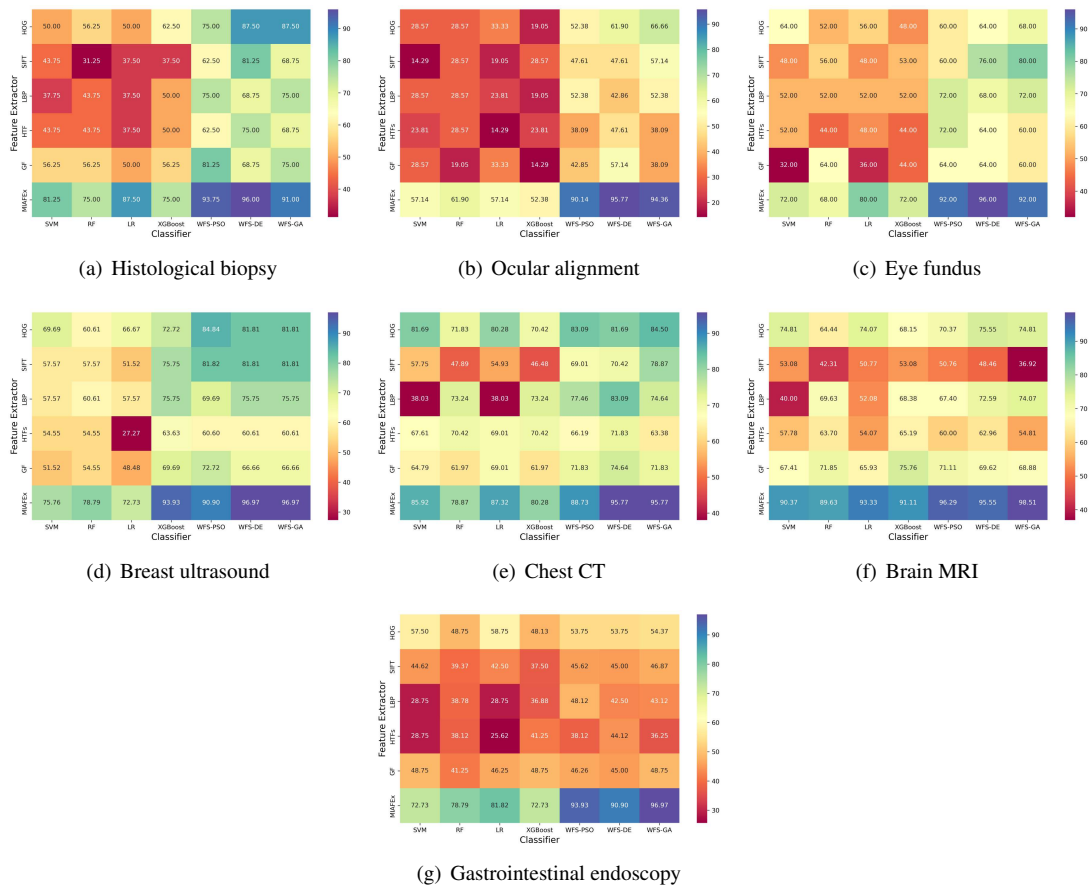


Figure 10: Accuracy performance on different feature extractors and classifiers over all datasets.

The performance of MIAFEx as a feature extractor demonstrates a clear advantage over traditional methods across the different medical imaging datasets. In the Gastrointestinal Endoscopy dataset, the WFS-PSO method achieved 93.93% accuracy, significantly outperforming other techniques, including MIAFEx with SVM (72.73%) and traditional methods like HOG (57.50%) or LBP (28.75%). Similarly, WFS-DE and WFS-GA also provided strong results, reaching 90.90% and 96.97% accuracy, respectively. This trend is evident across other datasets as well. In Brain

MRI, WFS-GA with MIAFEx reached 98.51%, surpassing traditional methods and the MIAFEx-SVM combination (90.37%). The Chest CT dataset followed a similar pattern, where WFS-DE reached 95.77%, WFS-GA achieved 95.77%, and MIAFEx with SVM yielded 85.92%, highlighting the effectiveness between WFS methods and MIAFEx in boosting classification performance. In more challenging datasets like Strabismus, WFS-DE and WFS-GA achieved accuracies of 95.77% and 94.36%, respectively, while traditional methods like HOG and LBP performed at 28.57% and 28.57%. The Lymphoma dataset further emphasizes the strength of WFS methods, with WFS-DE and WFS-GA yielding accuracies of 96.00% and 91.00%, respectively, compared to MIAFEx with SVM (81.25%).

The dependence of classical descriptors on handcrafted heuristics, along with their susceptibility to noise and limited adaptability, significantly reduced their effectiveness in all datasets. The results of this study demonstrate the superiority of MIAFEx as a feature extractor for various medical imaging tasks and its combination with ML classifiers and optimization techniques presents a promising approach for improving diagnostic accuracy in medical image analysis. While the absolute performance varies across domains, the trend remains consistent, remarking the MIAFEx as a superior feature extraction approach. Moreover, the use of optimization techniques (WFS-PSO, WFS-DE, WFS-GA) further improved the overall performance.

### 5.2. MIAFEx and DL models performance comparison

First, the training performance of the MIAFEx and the DL models is compared through its loss curves to provide insights into the optimization behavior and convergence rates of each method. Figure 11 illustrates the training loss curves for MIAFEx and the tested DL models across all the datasets.

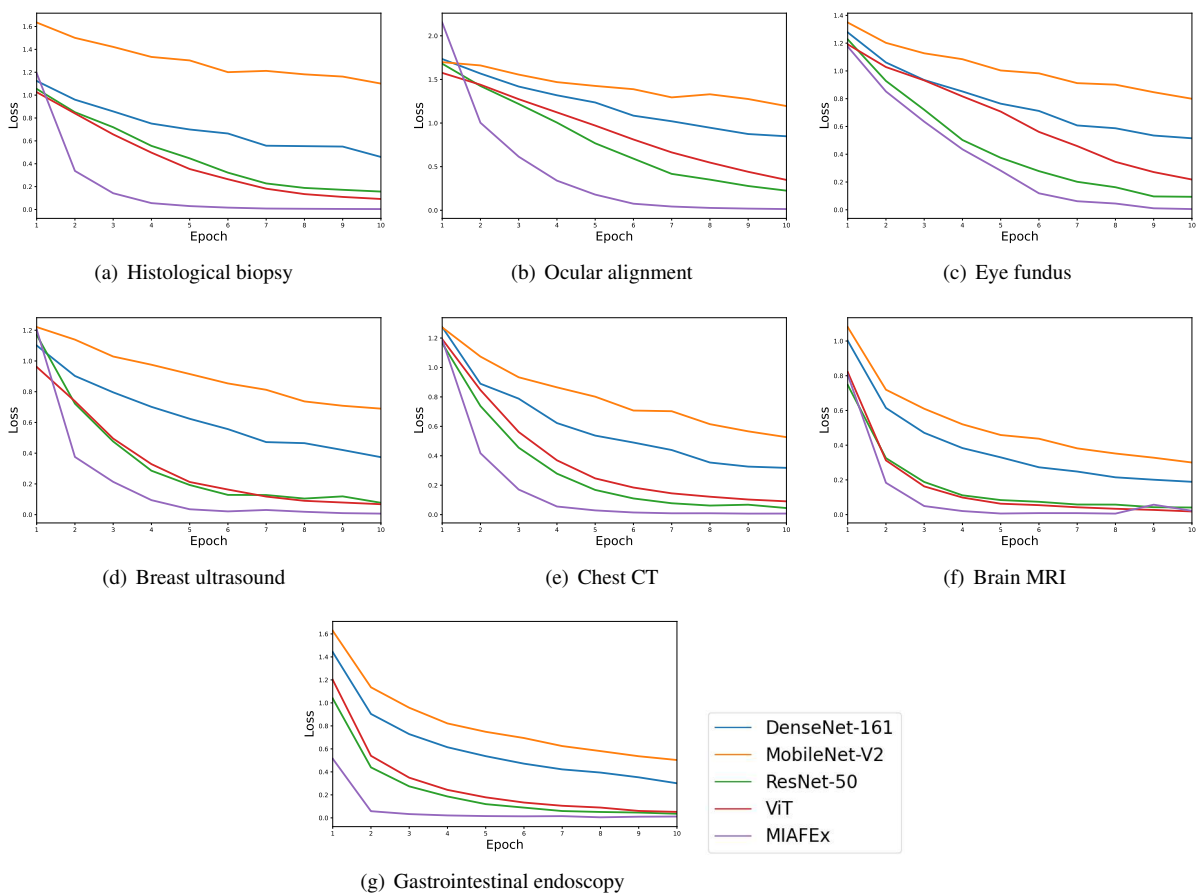


Figure 11: Training loss curves of the tested models and MIAFEx.



Notably, MIAFEx demonstrates a rapid convergence across all datasets, reflecting its capacity to effectively learn discriminative features even in the presence of limited training data. In contrast, the curves for conventional DL models, such as MobileNet-V2 and ResNet-50, exhibit slower convergence and higher variability, particularly on smaller datasets like Histological Biopsy and Ocular Alignment. This suggests that these models are more prone to overfitting in these datasets. Moreover, the lower final loss values achieved by MIAFEx across most datasets underline its robustness and ability to capture salient features with minimal residual error. In larger datasets, such as Brain MRI and Gastrointestinal Endoscopy, models like DenseNet-161 and ViT demonstrate competitive performance, with loss curves nearing those of MIAFEx. However, MIAFEx maintains a slight edge in achieving faster convergence, indicating its efficiency in adapting to diverse datasets.

Then, the performance of various DL models was evaluated and compared against the MIAFEx along different ML classifiers. The results, summarized in Tables 4 and 5, provide information regarding the performance of these models in different dataset sizes.

Table 4: Performance results of tested models on different datasets.

Dataset	Method	Accuracy	Precision	Recall	F1-Score
Histological biopsy	MobileNet-V2	69.63	70.78	69.69	70.02
	DenseNet-161	75.00	76.31	75.00	75.31
	ResNet-50	84.42	85.09	84.21	83.70
	ViT	67.76	67.94	67.76	66.75
	MIAFEx + LR	87.50	90.62	87.50	86.83
	MIAFEx + RF	75.00	77.08	75.00	73.40
	MIAFEx + SVM	81.25	82.81	81.25	80.75
	MIAFEx + XGBoost	75.00	77.08	75.00	73.40
	MIAFEx + WFS-PSO	93.75	94.64	93.75	93.64
	MIAFEx + WFS-DE	<b>96.00</b>	<b>96.29</b>	<b>96.00</b>	<b>95.79</b>
MIAFEx + WFS-GA	92.00	93.07	92.00	90.95	
Ocular alignment	MobileNet-V2	55.88	57.66	55.88	53.76
	DenseNet-161	58.82	63.27	58.82	59.13
	ResNet-50	68.62	70.22	68.62	68.73
	ViT	69.60	69.81	69.60	69.52
	MIAFEx + LR	57.14	66.55	57.14	56.60
	MIAFEx + RF	61.90	49.39	61.90	54.76
	MIAFEx + SVM	57.14	61.24	52.38	50.18
	MIAFEx + XGBoost	52.38	60.00	52.38	51.32
	MIAFEx + WFS-PSO	90.14	90.79	90.14	90.13
	MIAFEx + WFS-DE	<b>95.77</b>	<b>96.08</b>	<b>95.77</b>	<b>95.68</b>
MIAFEx + WFS-GA	94.36	94.47	94.37	94.37	
Eye fundus	MobileNet-V2	58.67	62.25	58.67	59.67
	DenseNet-161	61.15	63.86	61.15	62.11
	ResNet-50	62.80	62.01	62.80	62.18
	ViT	67.76	67.94	67.76	66.75
	MIAFEx + LR	80.00	83.00	80.00	79.42
	MIAFEx + RF	68.00	73.80	68.00	63.37
	MIAFEx + SVM	72.00	64.71	72.00	66.17
	MIAFEx + XGBoost	72.00	61.60	72.00	66.17
	MIAFEx + WFS-PSO	92.00	93.07	92.00	91.71
	MIAFEx + WFS-DE	<b>96.00</b>	<b>96.29</b>	<b>96.00</b>	<b>95.79</b>
MIAFEx + WFS-GA	92.00	93.07	92.00	90.95	
Breast ultrasound	MobileNet-V2	67.70	80.35	67.70	68.02
	DenseNet-161	80.74	83.07	80.74	81.26
	ResNet-50	85.71	86.31	85.71	85.86
	ViT	92.54	92.54	92.54	92.54
	MIAFEx + LR	81.82	81.85	81.82	81.11
	MIAFEx + RF	78.79	84.50	78.79	76.76
	MIAFEx + SVM	75.76	78.16	75.76	74.52
	MIAFEx + XGBoost	72.73	72.73	72.73	72.73
	MIAFEx + WFS-PSO	93.93	94.09	93.94	93.81
	MIAFEx + WFS-DE	90.90	90.90	90.90	90.90
MIAFEx + WFS-GA	<b>96.97</b>	<b>96.97</b>	<b>97.27</b>	<b>96.88</b>	

Table 5: Performance results of tested models on different datasets.

Dataset	Method	Accuracy	Precision	Recall	F1-Score
Chest CT	MobileNet-V2	72.59	72.26	72.59	72.96
	DenseNet-161	86.15	86.45	86.15	86.19
	ResNet-50	87.00	88.89	87.00	87.10
	ViT	80.22	80.91	80.22	80.00
	MIAFEx + LR	87.32	87.54	87.32	87.11
	MIAFEx + RF	78.87	82.38	78.87	78.22
	MIAFEx + SVM	85.92	78.43	76.06	76.02
	MIAFEx + XGBoost	80.28	82.09	80.28	79.87
	MIAFEx + WFS-PSO	88.73	90.04	88.73	88.86
	MIAFEx + WFS-DE	<b>95.77</b>	<b>95.98</b>	<b>95.77</b>	<b>95.78</b>
MIAFEx + WFS-GA	<b>95.77</b>	<b>96.20</b>	<b>95.77</b>	<b>95.78</b>	
Brain MRI	MobileNet-V2	94.06	94.10	94.06	94.01
	DenseNet-161	97.32	97.32	97.32	97.32
	ResNet-50	96.88	96.88	96.88	96.88
	ViT	97.32	97.32	97.32	97.32
	MIAFEx + LR	93.33	93.61	93.37	93.27
	MIAFEx + RF	89.63	89.67	89.63	89.59
	MIAFEx + SVM	90.37	90.74	90.37	90.37
	MIAFEx + XGBoost	91.11	91.36	91.11	91.36
	MIAFEx + WFS-PSO	96.29	96.29	96.29	96.29
	MIAFEx + WFS-DE	95.55	95.55	95.55	95.55
MIAFEx + WFS-GA	<b>98.51</b>	<b>98.51</b>	<b>98.51</b>	<b>98.51</b>	
Gastrointestinal endoscopy	MobileNet-V2	91.75	91.78	91.75	91.70
	DenseNet-161	92.62	92.67	92.62	92.59
	ResNet-50	92.12	92.34	92.12	92.12
	ViT	<b>93.25</b>	<b>93.29</b>	<b>93.25</b>	<b>93.25</b>
	MIAFEx + LR	88.12	88.94	88.12	88.16
	MIAFEx + RF	76.88	77.17	76.88	76.52
	MIAFEx + SVM	81.88	81.70	81.88	81.58
	MIAFEx + XGBoost	75.00	75.63	75.00	75.04
	MIAFEx + WFS-PSO	83.75	84.98	83.75	83.50
	MIAFEx + WFS-DE	88.12	88.36	88.12	88.03
MIAFEx + WFS-GA	87.50	88.63	87.50	87.19	

The results indicate that optimized models, particularly those using the MIAFEx framework combined with WFS-based algorithms (DE and GA), consistently outperform CNNs and ViT across multiple medical imaging datasets. This pattern is especially prominent in smaller datasets, such as histological biopsy and ocular alignment, where MIAFEx with optimization achieves notably high accuracies (up to 96%) compared to the other models. For datasets with larger sample sizes, such as chest CT and brain MRI, ViT presents a competitive or even superior performance, but its performance is still below WFS-based methods. However, when the dataset size reaches 4000 images, the ViT model reaches higher performance than MIAFEx-based ones, suggesting that attention mechanisms in ViTs are highly effective for capturing complex textures in large datasets.

Across all tested datasets, models using WFS-DE and WFS-GA optimizations maintain robust Precision, Recall, and F1-scores, emphasizing that feature selection through optimization significantly enhances model reliability in diverse imaging tasks. Overall, the combination of feature extraction and optimization proves advantageous, particularly in smaller datasets, while ViTs offer an alternative for large-scale medical datasets.

### 5.3. Dataset size performance analysis

To further study the impact of the dataset size on the tested models, the results in Fig. 12 provide an analysis of the accuracy performance of tested models across different dataset sizes.

For smaller datasets, particularly those with fewer than 1000 samples, the MIAFEx-based approaches demonstrate significantly higher performance compared to traditional models like MobileNet-V2, DenseNet-161, ResNet-50, and even the ViT model. For instance, with just 374 samples, MIAFEx with PSO achieves an impressive accuracy of 96%, while the highest-performing CNN, ResNet-50, only reaches 84.42%. This trend continues with datasets of 504 and 601 samples, where MIAFEx-based methods consistently outperform the CNNs and ViT, showcasing MIAFEx's

capability to provide great resources on limited data effectively. However, as the dataset size increases beyond approximately 1000 samples, the performance trend changes. Larger datasets see traditional CNNs and ViT start to yield superior accuracy, with DenseNet-161 and ViT achieving accuracies of 97.32% and 93.25% respectively at the 3362 images, but still being surpassed by MIAFEx + WFS-GA. When the dataset size reaches 4000 images, the ViT model and CNNs outperform all MIAFEx-based models. This suggests that while MIAFEx excels in scenarios with smaller datasets, the larger datasets provide sufficient information for DL models to optimize their architectures and learning capacities, hence achieving greater overall accuracy.

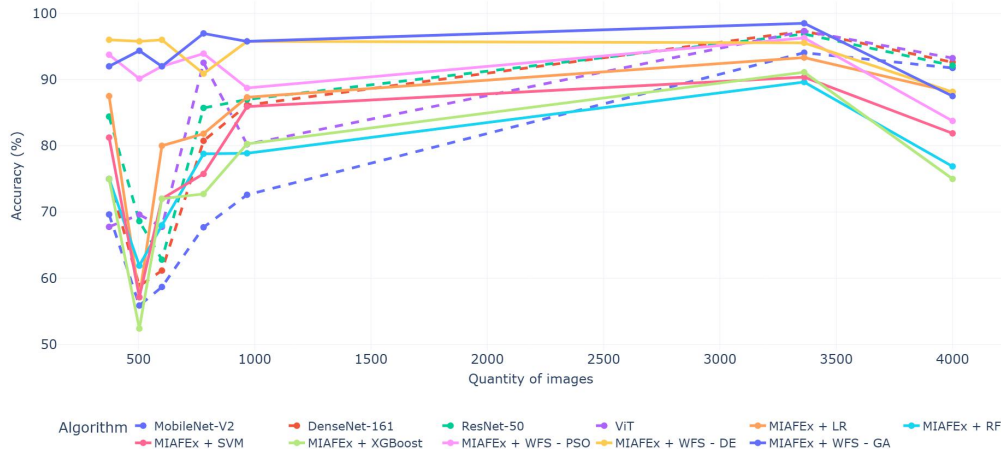


Figure 12: Classification performance of tested models on different image numbers.

These findings suggest that MIAFEx offers an efficient approach for applications with smaller medical datasets, while DL models remain advantageous when datasets include a large image quantity. This comparison highlights the importance of dataset size in model selection and suggests that a hybrid approach might be beneficial. Applying MIAFEx for smaller medical datasets provides higher performance than traditional feature extractors and DL models.

## 6. Conclusions

The paper introduces the MIAFEx, a novel attention-based feature extraction method specifically designed to address dataset-related challenges in medical image classification. By using a refinement mechanism within the transformer encoder, MIAFEx optimizes the classification token to focus on the most relevant features of medical images. This approach addresses limitations of both classical feature extraction techniques and modern deep learning models, particularly in scenarios with limited training data, and high intra-class variability, which are common in medical imaging.

Through comprehensive experiments across diverse medical imaging datasets, MIAFEx demonstrates notable improvements in accuracy, precision, recall, and F1-score over traditional feature extractors and popular DL methods, including CNNs and ViT. The integration of metaheuristic optimization techniques with MIAFEx further enhances classification performance, particularly in small datasets where standard models often struggle with overfitting. However, as expected, when larger datasets are available, CNNs and ViT models surpass MIAFEx in performance due to their capacity to learn more complex representations with increased data. This finding underscores the importance of dataset size in model selection, where MIAFEx is ideally suited for smaller datasets, while CNNs and ViTs are more effective with larger data.

In conclusion, MIAFEx proves to be an effective and versatile feature extraction method for medical image classification, with significant potential for early disease detection and diagnostic applications, setting a new benchmark for feature extraction in the field. Its ability to outperform existing methods on limited data suggests that MIAFEx could be highly impactful in real-world medical settings where data scarcity and variability are prevalent. Future work could explore further enhancements, scalability to larger datasets, and applicability across additional medical imaging domains.

## Appendix A. Performance of classical feature extractors and MIAFEx performance with ML classifiers

Table A.6: Performance on feature extraction on the histological biopsy dataset.

SVM					RF				
Feature extractor	Accuracy	Precision	Recall	F1-Score	Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	50.00	50.00	50.00	46.91	HOG	56.25	87.41	54.44	53.70
SIFT	43.75	42.97	43.75	41.51	SIFT	31.25	35.04	31.25	32.85
LBP	37.75	14.06	37.50	20.45	LBP	43.75	29.95	43.75	35.40
HTFs	43.75	45.83	43.33	42.10	Haralick	43.75	42.06	43.33	41.90
GF	56.25	56.25	56.25	56.25	Gabor	56.25	54.17	56.25	54.24
MIAFEx	<b>81.25</b>	<b>82.81</b>	<b>81.25</b>	<b>80.75</b>	MIAFEx	<b>75.00</b>	<b>77.08</b>	<b>75.00</b>	<b>73.40</b>

LR					XGBoost				
Feature extractor	Accuracy	Precision	Recall	F1-Score	Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	50.00	50.00	50.00	46.91	HOG	62.50	61.56	62.50	57.89
SIFT	37.50	38.54	37.50	35.62	SIFT	37.50	41.19	3.89	39.39
LBP	37.50	14.06	33.33	20.45	LBP	50.00	50.00	50.00	45.83
HTFs	37.50	29.17	37.50	32.14	Haralick	50.00	51.52	50.00	49.97
GF	50.00	50.52	50.00	48.65	Gabor	56.25	54.24	56.25	55.02
MIAFEx	<b>87.50</b>	<b>90.62</b>	<b>87.50</b>	<b>86.83</b>	MIAFEx	<b>75.00</b>	<b>77.08</b>	<b>75.00</b>	<b>73.40</b>

WFS-PSO					WFS-DE				
Feature extractor	Accuracy	Precision	Recall	F1-Score	Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	75.00	82.29	75.00	68.83	HOG	87.50	89.43	87.50	86.46
SIFT	62.50	59.38	62.50	57.68	SIFT	81.25	88.28	81.25	81.57
LBP	75.00	86.11	75.00	75.76	LBP	68.75	71.29	68.75	68.94
HTFs	62.50	58.04	62.50	59.39	Haralick	75.00	77.08	75.00	75.57
GF	81.25	81.77	81.25	81.06	Gabor	68.75	68.75	68.75	68.75
MIAFEx	<b>93.75</b>	<b>94.64</b>	<b>93.75</b>	<b>93.64</b>	MIAFEx	<b>96.00</b>	<b>96.29</b>	<b>96.00</b>	<b>95.79</b>

WFS-GA				
Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	87.50	91.07	87.50	86.98
SIFT	68.75	73.44	68.75	68.97
LBP	75.00	79.17	75.00	75.45
HTFs	68.75	69.79	68.78	67.95
GF	75.00	77.08	75.00	75.57
MIAFEx	<b>91.00</b>	<b>93.07</b>	<b>92.00</b>	<b>90.95</b>

Table A.7: Performance on feature extraction on the ocular alignment dataset.

SVM					RF				
Feature extractor	Accuracy	Precision	Recall	F1-Score	Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	28.57	21.43	26.00	23.05	HOG	28.57	16.89	26.00	20.32
SIFT	14.29	15.83	14.29	13.82	SIFT	28.57	22.59	28.57	25.13
LBP	28.57	17.78	28.00	17.27	LBP	28.57	34.00	28.00	30.00
HTFs	23.81	34.29	23.81	25.32	HTFs	28.57	22.04	28.57	24.87
GF	28.57	21.27	28.57	23.96	GF	19.05	22.22	19.05	19.77
MIAFEx	<b>57.14</b>	<b>61.24</b>	<b>52.38</b>	<b>50.18</b>	MIAFEx	<b>61.90</b>	<b>49.39</b>	<b>61.90</b>	<b>54.76</b>

LR					XGBoost				
Feature extractor	Accuracy	Precision	Recall	F1-Score	Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	33.33	24.76	31.00	27.33	HOG	19.05	17.52	18.00	17.35
SIFT	19.05	31.09	19.05	20.19	SIFT	28.57	32.54	28.57	27.85
LBP	23.81	9.90	23.00	13.71	LBP	19.05	24.00	19.00	20.67
HTFs	14.29	22.00	13.00	14.28	HTFs	23.81	19.44	23.00	20.71
GF	33.33	31.22	33.33	31.03	GF	14.29	13.33	13.00	12.89
MIAFEx	<b>57.14</b>	<b>66.55</b>	<b>57.14</b>	<b>56.60</b>	MIAFEx	<b>52.38</b>	<b>60.00</b>	<b>52.38</b>	<b>51.32</b>

WFS-PSO					WFS-DE				
Feature extractor	Accuracy	Precision	Recall	F1-Score	Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	52.38	50.58	52.38	48.53	HOG	61.90	51.93	91.90	54.31
SIFT	47.61	59.41	47.62	45.77	SIFT	47.61	86.03	47.62	48.97
LBP	52.38	50.79	52.38	50.88	LBP	42.86	41.27	42.86	38.49
HTFs	38.09	36.51	38.10	36.28	HTFs	47.61	56.26	47.62	45.81
GF	42.85	46.35	42.86	43.65	GF	57.14	57.86	57.14	55.87
MIAFEx	<b>90.14</b>	<b>90.79</b>	<b>90.14</b>	<b>90.13</b>	MIAFEx	<b>95.77</b>	<b>96.08</b>	<b>95.77</b>	<b>95.68</b>

WFS-GA				
Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	66.66	57.14	66.67	60.31
SIFT	57.14	79.89	57.14	52.67
LBP	52.38	63.72	52.38	48.26
HTFs	38.09	52.15	38.10	38.82
GF	38.09	39.12	38.10	36.84
MIAFEx	<b>94.36</b>	<b>94.47</b>	<b>94.37</b>	<b>94.37</b>

Table A.8: Performance on feature extraction on the eye fundus dataset.

SVM					RF				
Feature extractor	Accuracy	Precision	Recall	F1-Score	Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	64.00	62.73	64.00	55.70	HOG	52.00	27.04	52.00	35.58
SIFT	48.00	41.25	48.00	43.81	SIFT	56.00	43.78	56.00	48.90
LBP	52.00	27.04	52.00	35.58	LBP	52.00	50.58	52.00	50.56
HTFs	52.00	27.04	52.00	35.58	HTFs	44.00	38.00	44.00	40.96
GF	32.00	32.53	32.00	32.13	GF	64.00	56.84	64.00	58.05
MIAFEx	<b>72.00</b>	<b>64.71</b>	<b>72.00</b>	<b>67.31</b>	MIAFEx	<b>68.00</b>	<b>73.80</b>	<b>68.00</b>	<b>63.37</b>

LR					XGBoost				
Feature extractor	Accuracy	Precision	Recall	F1-Score	Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	56.00	44.17	56.00	42.94	HOG	48.00	38.04	48.00	41.64
SIFT	48.00	38.59	48.00	42.67	SIFT	53.00	44.89	52.00	47.26
LBP	52.00	27.04	52.00	35.58	LBP	52.00	50.58	52.00	50.56
HTFs	48.00	36.00	48.00	33.73	HTFs	44.00	37.38	44.00	40.67
GF	36.00	34.00	36.00	34.02	GF	44.00	48.27	44.00	45.05
MIAFEx	<b>80.00</b>	<b>83.00</b>	<b>80.00</b>	<b>79.42</b>	MIAFEx	<b>72.00</b>	<b>61.60</b>	<b>72.00</b>	<b>66.17</b>

WFS-PSO					WFS-DE				
Feature extractor	Accuracy	Precision	Recall	F1-Score	Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	60.00	68.20	60.00	62.65	HOG	64.00	60.84	64.00	57.40
SIFT	60.00	42.44	60.00	49.70	SIFT	76.00	66.43	76.00	68.53
LBP	72.00	73.67	72.00	71.95	LBP	68.00	65.05	68.00	65.35
HTFs	72.00	73.56	72.00	67.35	HTFs	64.00	54.67	64.00	57.59
GF	64.00	57.87	64.00	58.04	GF	64.00	68.99	64.00	61.32
MIAFEx	<b>92.00</b>	<b>93.07</b>	<b>92.00</b>	<b>90.95</b>	MIAFEx	<b>96.00</b>	<b>96.29</b>	<b>96.00</b>	<b>95.79</b>

WFS-GA				
Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	68.00	70.98	68.00	67.09
SIFT	80.00	85.14	80.00	80.02
LBP	72.00	74.00	72.00	70.01
HTFs	60.00	58.11	60.00	54.15
GF	60.00	50.10	60.00	54.53
MIAFEx	<b>92.00</b>	<b>93.07</b>	<b>92.00</b>	<b>90.95</b>

Table A.9: Performance on feature extraction on the breast ultrasound dataset.

SVM					RF				
Feature extractor	Accuracy	Precision	Recall	F1-Score	Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	69.69	72.64	69.69	69.06	HOG	60.61	61.46	60.61	48.35
SIFT	57.57	47.76	57.57	50.96	SIFT	57.57	47.76	57.57	50.96
LBP	57.57	33.15	57.57	42.07	LBP	60.61	64.77	60.61	58.08
HTFs	54.55	32.39	54.55	40.64	HTFs	54.55	54.55	54.55	53.94
GF	51.52	52.53	51.51	51.95	GF	54.55	55.56	54.55	54.49
MIAFEx	<b>75.76</b>	<b>78.16</b>	<b>75.76</b>	<b>74.52</b>	MIAFEx	<b>78.79</b>	<b>84.50</b>	<b>78.79</b>	<b>76.76</b>

LR					XGBoost				
Feature extractor	Accuracy	Precision	Recall	F1-Score	Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	66.67	70.33	66.67	66.36	HOG	66.67	70.98	66.67	63.10
SIFT	57.57	47.76	57.58	50.96	SIFT	51.52	42.47	51.52	46.26
LBP	57.57	33.15	57.57	42.07	LBP	57.57	59.18	57.57	57.94
HTFs	48.48	47.14	48.48	42.60	HTFs	27.27	31.28	27.27	28.58
GF	51.52	54.51	51.52	52.58	GF	48.48	55.53	48.48	49.70
MIAFEx	<b>81.82</b>	<b>81.85</b>	<b>81.82</b>	<b>81.11</b>	MIAFEx	<b>72.73</b>	<b>72.73</b>	<b>72.73</b>	<b>72.73</b>

WFS-PSO					WFS-DE				
Feature extractor	Accuracy	Precision	Recall	F1-Score	Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	72.72	76.52	72.73	72.29	HOG	84.84	86.09	84.85	83.91
SIFT	75.75	64.45	75.75	69.07	SIFT	81.82	71.03	81.82	75.39
LBP	75.75	79.95	75.75	71.85	LBP	69.69	75.35	69.69	65.69
HTFs	63.63	57.47	63.63	56.69	HTFs	60.60	49.89	60.61	53.47
GF	69.69	60.89	69.70	62.14	GF	72.72	81.94	72.72	68.84
MIAFEx	<b>93.93</b>	<b>94.09</b>	<b>93.94</b>	<b>93.81</b>	MIAFEx	<b>90.90</b>	<b>90.90</b>	<b>90.90</b>	<b>90.90</b>

WFS-GA				
Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	81.81	84.34	81.82	78.69
SIFT	81.81	83.93	81.82	78.35
LBP	75.75	79.33	75.76	73.95
HTFs	60.61	58.22	60.61	55.41
GF	66.66	58.18	66.66	58.17
MIAFEx	<b>96.97</b>	<b>96.97</b>	<b>97.27</b>	<b>96.88</b>

Table A.10: Performance on feature extraction on the chest CT dataset.

SVM					RF				
Feature extractor	Accuracy	Precision	Recall	F1-Score	Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	81.69	82.53	81.69	81.15	HOG	71.83	71.03	71.83	69.49
SIFT	57.75	54.88	57.75	54.25	SIFT	47.89	38.49	47.89	41.25
LBP	38.03	14.46	38.03	20.95	LBP	73.24	74.17	73.24	72.49
HTFs	67.61	65.38	67.61	62.95	HTFs	70.42	68.92	70.42	69.15
GF	64.79	65.23	64.79	63..37	GF	61.97	60.10	61.97	58.59
MIAFEx	<b>85.92</b>	<b>86.34</b>	<b>85.92</b>	<b>85.88</b>	MIAFEx	<b>78.87</b>	<b>82.38</b>	<b>78.87</b>	<b>78.22</b>

LR					XGBoost				
Feature extractor	Accuracy	Precision	Recall	F1-Score	Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	80.28	81.73	80.28	79.75	HOG	70.42	68.87	70.42	69.16
SIFT	54.93	46.56	54.93	49.94	SIFT	46.48	39.69	46.48	42.20
LBP	38.03	16.04	38.03	22.57	LBP	73.24	73.66	73.24	72.45
HTFs	69.01	68.73	69.01	65.01	HTFs	70.42	69.79	70.42	70.01
GF	69.01	68.34	69.01	68.60	GF	61.97	60.15	61.97	60.28
MIAFEx	<b>87.32</b>	<b>87.54</b>	<b>87.32</b>	<b>87.11</b>	MIAFEx	<b>80.28</b>	<b>82.09</b>	<b>80.28</b>	<b>79.87</b>

WFS-PSO					WFS-DE				
Feature extractor	Accuracy	Precision	Recall	F1-Score	Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	83.09	83.40	83.10	82.58	HOG	81.69	82.25	81.69	81.23
SIFT	69.01	70.62	69.01	67.84	SIFT	70.42	73.69	70.42	68.48
LBP	77.46	78.87	77.46	77.59	LBP	83.09	83.34	83.10	82.90
HTFs	66.19	66.56	66.20	65.99	HTFs	71.83	74.05	71.83	69.49
GF	71.83	72.84	71.83	71.69	GF	74.64	74.85	74.65	74.72
MIAFEx	<b>88.73</b>	<b>90.04</b>	<b>88.73</b>	<b>88.86</b>	MIAFEx	<b>95.77</b>	<b>95.98</b>	<b>95.77</b>	<b>95.78</b>

WFS-GA				
Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	84.50	86.35	84.51	84.65
SIFT	78.87	81.99	78.87	77.02
LBP	74.64	74.80	74.65	74.63
HTFs	63.38	63.17	63.38	61.85
GF	71.83	71.15	71.83	70.49
MIAFEx	<b>95.77</b>	<b>96.20</b>	<b>95.77</b>	<b>95.78</b>



Table A.11: Performance on feature extraction on the brain MRI dataset.

SVM					RF				
Feature extractor	Accuracy	Precision	Recall	F1-Score	Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	74.81	74.65	74.81	74.17	HOG	64.44	68.85	64.44	62.55
SIFT	53.08	57.50	53.08	56.21	SIFT	42.31	43.68	43.21	39.96
LBP	40.00	42.78	40.00	33.79	LBP	69.63	69.44	69.63	69.22
HTFs	57.78	57.39	57.78	55.83	HTFs	63.70	64.42	63.70	63.65
GF	67.41	68.28	67.41	67.53	GF	71.85	71.61	71.85	71.50
MIAFEx	<b>90.37</b>	<b>90.74</b>	<b>90.37</b>	<b>90.37</b>	MIAFEx	<b>89.63</b>	<b>89.67</b>	<b>89.63</b>	<b>89.59</b>

LR					XGBoost				
Feature extractor	Accuracy	Precision	Recall	F1-Score	Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	74.07	74.14	74.07	73.64	HOG	68.15	67.31	68.15	66.87
SIFT	50.77	52.07	50.77	50.66	SIFT	53.08	57.64	53.08	52.02
LBP	52.08	59.98	54.81	53.01	LBP	68.38	67.46	68.15	67.56
HTFs	54.07	52.77	54.07	51.96	HTFs	65.19	65.93	65.19	65.34
GF	65.93	67.08	65.93	65.54	GF	75.76	75.21	75.56	75.20
MIAFEx	<b>93.33</b>	<b>93.61</b>	<b>93.37</b>	<b>93.27</b>	MIAFEx	<b>91.11</b>	<b>91.36</b>	<b>91.11</b>	<b>91.36</b>

WFS-PSO					WFS-DE				
Feature extractor	Accuracy	Precision	Recall	F1-Score	Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	70.37	71.61	70.37	69.82	HOG	75.55	78.46	75.45	75.26
SIFT	50.76	37.69	50.77	42.39	SIFT	48.46	35.73	48.46	41.03
LBP	67.40	70.43	67.41	68.28	LBP	72.59	73.42	72.59	72.90
HTFs	60.00	60.72	60.00	60.04	HTFs	62.96	67.74	62.96	63.85
GF	71.11	71.26	71.11	70.78	GF	69.62	70.76	69.63	69.20
MIAFEx	<b>96.29</b>	<b>96.29</b>	<b>96.29</b>	<b>96.29</b>	MIAFEx	<b>95.55</b>	<b>95.55</b>	<b>95.55</b>	<b>95.55</b>

WFS-GA				
Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	74.81	79.70	74.81	74.70
SIFT	36.92	52.14	36.91	31.43
LBP	74.07	74.12	74.07	74.07
HTFs	54.81	54.93	54.81	54.58
GF	68.88	70.94	68.89	69.15
MIAFEx	<b>98.51</b>	<b>98.51</b>	<b>98.51</b>	<b>98.51</b>

Table A.12: Performance on feature extraction on the gastrointestinal endoscopy dataset.

SVM					RF				
Feature extractor	Accuracy	Precision	Recall	F1-Score	Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	57.50	57.86	57.50	56.95	HOG	48.75	49.53	48.75	47.80
SIFT	44.62	44.86	45.62	44.19	SIFT	39.37	38.35	39.37	38.28
LBP	28.75	17.54	28.75	20.81	LBP	38.78	38.90	38.75	38.30
HTFs	28.75	26.35	28.75	26.42	HTFs	38.12	38.41	38.12	37.76
GF	48.75	49.02	48.75	48.00	GF	41.25	40.97.00	41.25	40.61
MIAFEx	<b>72.73</b>	<b>78.16</b>	<b>72.73</b>	<b>74.52</b>	MIAFEx	<b>78.79</b>	<b>84.50</b>	<b>78.79</b>	<b>76.76</b>

LR					XGBoost				
Feature extractor	Accuracy	Precision	Recall	F1-Score	Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	58.75	58.96	58.75	57.81	HOG	48.13	48.05	48.13	47.92
SIFT	42.50	43.32	42.50	41.59	SIFT	37.50	37.56	37.50	35.93
LBP	28.75	17.13	28.75	16.73	LBP	36.88	37.08	36.88	36.83
HTFs	25.62	24.57	25.63	24.39	HTFs	41.25	41.41	41.25	40.79
GF	46.25	44.58	46.25	45.13	GF	48.75	48.85	48.75	48.42
MIAFEx	<b>81.82</b>	<b>81.85</b>	<b>81.82</b>	<b>81.11</b>	MIAFEx	<b>72.73</b>	<b>72.73</b>	<b>72.73</b>	<b>72.73</b>

WFS-PSO					WFS-DE				
Feature extractor	Accuracy	Precision	Recall	F1-Score	Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	53.75	60.43	53.75	49.61	HOG	53.75	57.39	53.75	47.97
SIFT	45.62	44.52	45.62	41.38	SIFT	45.00	41.74	45.00	40.48
LBP	48.12	48.97	48.12	48.00	LBP	42.50	43.15	42.50	42.34
HTFs	38.12	38.41	38.12	37.26	HTFs	44.12	44.61	43.12	43.26
GF	46.26	49.94	46.25	45.25	GF	45.00	44.10	45.00	43.26
MIAFEx	<b>93.93</b>	<b>94.09</b>	<b>93.94</b>	<b>93.81</b>	MIAFEx	<b>90.90</b>	<b>90.90</b>	<b>90.90</b>	<b>90.90</b>

WFS-GA				
Feature extractor	Accuracy	Precision	Recall	F1-Score
HOG	54.37	60.66	54.37	50.13
SIFT	46.87	55.34	46.88	44.03
LBP	43.12	47.36	43.12	43.50
HTFs	36.25	36.10	36.25	34.90
GF	48.75	49.75	48.75	48.15
MIAFEx	<b>96.97</b>	<b>96.97</b>	<b>97.27</b>	<b>96.88</b>

## References

- [1] A. S. Pillai, Utilizing deep learning in medical image analysis for enhanced diagnostic accuracy and patient care: Challenges, opportunities, and ethical implications, *Journal of Deep Learning in Genomic Data Analysis* 1 (1) (2021) 1–17.
- [2] Z. Ahmed, K. Mohamed, S. Zeeshan, X. Dong, Artificial intelligence with multi-functional machine learning platform development for better healthcare and precision medicine, *Database* 2020 (2020) baaa010.
- [3] M. Rana, M. Bhushan, Machine learning and deep learning approach for medical image analysis: diagnosis to detection, *Multimedia Tools and Applications* 82 (17) (2023) 26731–26769.
- [4] G. Calderon-Auza, C. Carrillo-Gomez, M. Nakano, K. Toscano-Medina, H. Perez-Meana, A. Gonzalez-H. Leon, H. Quiroz-Mercado, A teleophthalmology support system based on the visibility of retinal elements using the cnns, *Sensors* 20 (10) (2020) 2838.
- [5] Q. An, S. Rahman, J. Zhou, J. J. Kang, A comprehensive review on machine learning in healthcare industry: classification, restrictions, opportunities and challenges, *Sensors* 23 (9) (2023) 4178.
- [6] D. Karimi, H. Dou, S. K. Warfield, A. Gholipour, Deep learning with noisy labels: Exploring techniques and remedies in medical image analysis, *Medical image analysis* 65 (2020) 101759.
- [7] D. Tsipras, S. Santurkar, L. Engstrom, A. Ilyas, A. Madry, From imagenet to image classification: Contextualizing progress on benchmarks, in: *International Conference on Machine Learning*, PMLR, 2020, pp. 9625–9635.
- [8] M. Nixon, A. Aguado, Feature extraction and image processing for computer vision, Academic press, 2019.
- [9] Z. Li, X. Zhang, H. Müller, S. Zhang, Large-scale retrieval for medical image analytics: A comprehensive review, *Medical image analysis* 43 (2018) 66–84.
- [10] S. Routray, A. K. Ray, C. Mishra, Analysis of various image feature extraction methods against noisy image: Sift, surf and hog, in: *2017 Second International Conference on Electrical, Computer and Communication Technologies (ICECCT)*, IEEE, 2017, pp. 1–5.
- [11] Z. Li, K. Kamnitsas, B. Glocker, Analyzing overfitting under class imbalance in neural networks for image segmentation, *IEEE transactions on medical imaging* 40 (3) (2020) 1065–1077.
- [12] M. Sarah, L. Mathieu, Z. Philippe, A. L. Guilcher, L. Borderie, B. Cochener, G. Quellec, Generalizing deep learning models for medical image classification, *arXiv preprint arXiv:2403.12167* (2024).
- [13] D. M. Hawkins, The problem of overfitting, *Journal of chemical information and computer sciences* 44 (1) (2004) 1–12.
- [14] M. El-Gayar, H. Soliman, et al., A comparative study of image low level feature extraction algorithms, *Egyptian Informatics Journal* 14 (2) (2013) 175–181.
- [15] D.-C. He, L. Wang, Texture unit, texture spectrum, and texture analysis, *IEEE transactions on Geoscience and Remote Sensing* 28 (4) (1990) 509–512.
- [16] N. Dalal, B. Triggs, Histograms of oriented gradients for human detection, in: *2005 IEEE computer society conference on computer vision and pattern recognition (CVPR'05)*, Vol. 1, Ieee, 2005, pp. 886–893.
- [17] C. L. Chowdhary, D. P. Acharjya, Segmentation and feature extraction in medical imaging: a systematic review, *Procedia Computer Science* 167 (2020) 26–36.
- [18] T. J. Alhindi, S. Kalra, K. H. Ng, A. Afrin, H. R. Tizhoosh, Comparing lbp, hog and deep features for classification of histopathology images, in: *2018 international joint conference on neural networks (IJCNN)*, IEEE, 2018, pp. 1–7.
- [19] A. Liebgott, T. Küstner, H. Strohmeier, T. Hepp, P. Mangold, P. Martirosian, F. Bamberg, K. Nikolaou, B. Yang, S. Gatidis, Imfeatbox: a toolbox for extraction and analysis of medical image features, *International journal of computer assisted radiology and surgery* 13 (2018) 1881–1893.
- [20] R. J. S. Raj, S. J. Shobana, I. V. Pustokhina, D. A. Pustokhin, D. Gupta, K. Shankar, Optimal feature selection-based medical image classification using deep learning model in internet of medical things, *IEEE Access* 8 (2020) 58006–58017.
- [21] A. RV, S. AP, Augmenting transfer learning with feature extraction techniques for limited breast imaging datasets, *Journal of Digital Imaging* 34 (3) (2021) 618–629.
- [22] O. O. Akinola, A. E. Ezugwu, J. O. Agushaka, R. A. Zitar, L. Abualigah, Multiclass feature selection with metaheuristic optimization algorithms: a review, *Neural Computing and Applications* 34 (22) (2022) 19751–19790.
- [23] G. Nagarajan, R. Minu, B. Muthukumar, V. Vedanarayanan, S. Sundarsingh, Hybrid genetic algorithm for medical image feature extraction and selection, *Procedia Computer Science* 85 (2016) 455–462.
- [24] S. EcheGARAY, S. Bakr, D. L. Rubin, S. Napel, Quantitative image feature engine (qife): an open-source, modular engine for 3d quantitative feature extraction from volumetric medical images, *Journal of digital imaging* 31 (2018) 403–414.
- [25] F. H. Kuwil, A new feature extraction approach of medical image based on data distribution skew, *Neuroscience Informatics* 2 (3) (2022) 100097.
- [26] A. K. Sharma, A. Nandal, A. Dhaka, K. Polat, R. Alwadie, F. Alenezi, A. Alhudhaif, Hog transformation based feature extraction framework in modified resnet50 model for brain tumor detection, *Biomedical Signal Processing and Control* 84 (2023) 104737.
- [27] V. Narayan, P. K. Mall, S. Awasthi, S. Srivastava, A. Gupta, Fuzzynet: Medical image classification based on glcm texture feature, in: *2023 International Conference on Artificial Intelligence and Smart Communication (AISC)*, IEEE, 2023, pp. 769–773.
- [28] Y. H. Liu, Feature extraction and image recognition with convolutional neural networks, in: *Journal of Physics: Conference Series*, Vol. 1087, IOP Publishing, 2018, p. 062032.
- [29] J. Kim, K. Shim, J. Kim, B. Shim, Vision transformer-based feature extraction for generalized zero-shot learning, in: *ICASSP 2023-2023 IEEE International Conference on Acoustics, Speech and Signal Processing (ICASSP)*, IEEE, 2023, pp. 1–5.
- [30] J. Li, J. Chen, Y. Tang, C. Wang, B. A. Landman, S. K. Zhou, Transforming medical imaging with transformers? a comparative review of key properties, current progresses, and future perspectives, *Medical image analysis* 85 (2023) 102762.
- [31] S. Takahashi, Y. Sakaguchi, N. Kouno, K. Takasawa, K. Ishizu, Y. Akagi, R. Aoyama, N. Teraya, A. Bolatkan, N. Shinkai, et al., Comparison of vision transformers and convolutional neural networks in medical image analysis: A systematic review, *Journal of Medical Systems* 48 (1) (2024) 1–22.

- [32] J. W. Kim, A. U. Khan, I. Banerjee, Systematic review of hybrid vision transformer architectures for radiological image analysis, *medRxiv* (2024) 2024-06.
- [33] O. N. Manzari, H. Ahmadabadi, H. Kashiani, S. B. Shokouhi, A. Ayatollahi, Medvit: a robust vision transformer for generalized medical image classification, *Computers in Biology and Medicine* 157 (2023) 106791.
- [34] W. Ding, H. Wang, J. Huang, H. Ju, Y. Geng, C.-T. Lin, W. Pedrycz, Ftrascnn: Fusing transformer and a cnn based on fuzzy logic for uncertain medical image segmentation, *Information Fusion* 99 (2023) 101880.
- [35] X. Huo, G. Sun, S. Tian, Y. Wang, L. Yu, J. Long, W. Zhang, A. Li, Hifuse: Hierarchical multi-scale feature fusion network for medical image classification, *Biomedical Signal Processing and Control* 87 (2024) 105534.
- [36] Y. Yue, Z. Li, Medmamba: Vision mamba for medical image classification, *arXiv preprint arXiv:2403.03849* (2024).
- [37] A. Dosovitskiy, An image is worth 16x16 words: Transformers for image recognition at scale, *arXiv preprint arXiv:2010.11929* (2020).
- [38] W. Al-Dhabyani, M. Gomaa, H. Khaled, A. Fahmy, Dataset of breast ultrasound images, *Data in brief* 28 (2020) 104863.
- [39] T. Löfstedt, P. Brynolfsson, T. Asklund, T. Nyholm, A. Garpebring, Gray-level invariant haralick texture features, *PLoS one* 14 (2) (2019) e0212110.
- [40] Lee, Wang, Fingerprint feature extraction using gabor filters, *Electronics letters* 35 (4) (1999) 288–290.
- [41] P. Komarek, Logistic regression for data mining and high-dimensional classification, *Carnegie Mellon University*, 2004.
- [42] S. J. Rigatti, Random forest, *Journal of Insurance Medicine* 47 (1) (2017) 31–39.
- [43] M. A. Chandra, S. Bedi, Survey on svm and their application in image classification, *International Journal of Information Technology* 13 (5) (2021) 1–11.
- [44] T. Chen, Xgboost: extreme gradient boosting, *R package version 0.4-2* 1 (4) (2015).
- [45] R. A. Kumar, J. V. Franklin, N. Koppula, A comprehensive survey on metaheuristic algorithm for feature selection techniques, *Materials Today: Proceedings* 64 (2022) 435–441.
- [46] I. Miguel-Andrés, J. Ramos-Frutos, M. Sharawi, D. Oliva, E. Reyes-Dávila, Á. Casas-Ordaz, M. Pérez-Cisneros, S. Zapotecas-Martínez, Wrapper-based feature selection to classify flatfoot disease, *IEEE Access* (2024).
- [47] M. Sandler, A. Howard, M. Zhu, A. Zhmoginov, L.-C. Chen, Mobilenetv2: Inverted residuals and linear bottlenecks, in: *Proceedings of the IEEE conference on computer vision and pattern recognition*, 2018, pp. 4510–4520.
- [48] G. Huang, Z. Liu, L. Van Der Maaten, K. Q. Weinberger, Densely connected convolutional networks, in: *Proceedings of the IEEE conference on computer vision and pattern recognition*, 2017, pp. 4700–4708.
- [49] K. He, X. Zhang, S. Ren, J. Sun, Deep residual learning for image recognition, in: *Proceedings of the IEEE conference on computer vision and pattern recognition*, 2016, pp. 770–778.
- [50] J. Kennedy, R. Eberhart, Particle swarm optimization, in: *Proceedings of ICNN'95-international conference on neural networks*, Vol. 4, IEEE, 1995, pp. 1942–1948.
- [51] K. V. Price, Differential evolution: a fast and simple numerical optimizer, in: *Proceedings of North American fuzzy information processing*, IEEE, 1996, pp. 524–527.
- [52] J. H. Holland, Genetic algorithms, *Scientific american* 267 (1) (1992) 66–73.
- [53] T. Dozat, Incorporating nesterov momentum into adam, in: *In Proceedings of the 4th International Conference on Learning Representations*, 2016.
- [54] A. Mao, M. Mohri, Y. Zhong, Cross-entropy loss functions: Theoretical analysis and applications, in: *International conference on Machine learning*, PMLR, 2023, pp. 23803–23828.
- [55] L. Torrey, J. Shavlik, Transfer learning, in: *Handbook of research on machine learning applications and trends: algorithms, methods, and techniques*, IGI global, 2010, pp. 242–264.
- [56] J. Deng, W. Dong, R. Socher, L.-J. Li, K. Li, L. Fei-Fei, Imagenet: A large-scale hierarchical image database, in: *2009 IEEE conference on computer vision and pattern recognition*, Ieee, 2009, pp. 248–255.
- [57] T. Ridnik, E. Ben-Baruch, A. Noy, L. Zelnik-Manor, Imagenet-21k pretraining for the masses, *arXiv preprint arXiv:2104.10972* (2021).
- [58] B. Wu, C. Xu, X. Dai, A. Wan, P. Zhang, Z. Yan, M. Tomizuka, J. Gonzalez, K. Keutzer, P. Vajda, Visual transformers: Token-based image representation and processing for computer vision (2020). *arXiv:2006.03677*.
- [59] Y. You, Z. Zhang, C.-J. Hsieh, J. Demmel, K. Keutzer, Imagenet training in minutes, in: *Proceedings of the 47th international conference on parallel processing*, 2018, pp. 1–10.